

Version 8.0
May 2009

NICMOS Data Handbook

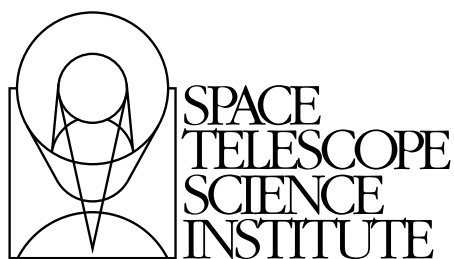

Hubble Division
3700 San Martin Drive
Baltimore, Maryland 21218
help@stsci.edu

User Support

For prompt answers to any question, please contact the STScI Help Desk.

- **E-mail:** help@stsci.edu
- **Phone:** (410) 338-1082
(800) 544-8125 (U.S., toll free)

World Wide Web

Information and other resources are available on the Web site:

- **URL:** <http://www.stsci.edu/hst/nicmos>.

Revision History

Version	Date	Editors
8.0	May 2009	Deepashri Thatte, Tomas Dahlen, Elizabeth Barker, Roelof de Jong, Anton Koekemoer, Nor Pirzkal, Alex Viana, Tommy Wiklind
7.0	April 2007	Helene McLaughlin & Tommy Wiklind et al.
6.0	July 2004	Bahram Mobasher & Erin Roye et al.
5.0	January 2002	Mark Dickinson et al.
4.0	December 1999	Mark Dickinson et al.
3.0	October 1997	Daniela Calzetti et al.

Acknowledgments

The editors are grateful for the contributions from the past and present members of the NICMOS group and members of the SSB group at STScI including: Santiago Arribas, Eddie Bergeron, Torsten Boeker, Howard Bushouse, Daniela Calzetti, Luis Colina, Mark Dickinson, Sherie Holfeltz, David Grumm, Chris Hanley, Robert Jedrzejewski, Victoria Laidler, Lisa Mazzuca, Helene McLaughlin, Bahram Mobasher, Keith Noll, Antonella Nota, Adam Riess, Erin Roye, Chris Skinner, Al Schultz, Anand Sivaramakrishnan, Megan Sosey, Alex Storrs, Anatoly Suchkov, Chun Xu, and Wolfram Freudling (ST-ECF). We are also grateful for technical assistance provided by Susan Rose and Jim Younger in editing this Handbook.

Citation:

In publications, refer to this document as:

Thatte, D. and Dahlen, T. et al. 2009, "NICMOS Data Handbook", version 8.0, (Baltimore, STScI)

Send comments or corrections to:
Hubble Division
Space Telescope Science Institute
3700 San Martin Drive
Baltimore, Maryland 21218
E-mail: help@stsci.edu

Table of Contents

List of Figures	vii
List of Tables	ix
Preface	xi
Chapter 1: Instrument Overview	1
1.1 Instrument Overview	1
1.2 Detector Readout Modes	4
1.2.1 MULTIACCUM	5
1.2.2 ACCUM	5
1.2.3 BRIGHTOBJ	6
1.2.4 RAMP	7
Chapter 2: Data Structures	9
2.1 NICMOS Data Files	9
2.1.1 File Name Suffixes	10
2.1.2 Science Data Files	12
2.1.3 Auxiliary Data Files	17
2.2 Header Keywords	19
2.3 Working with NICMOS Files	28
2.4 From the Phase II Proposal to Your Data	31
2.5 Paper Products	33
Chapter 3: Calibration	35
3.1 Pipeline Processing, OTFR, and the HST Archive	35
3.2 NICMOS Calibration Software	37
3.2.1 The Calibration Pipeline	37
3.2.2 Software for Grism Data Reduction	38

3.3 Basic Data Reduction.....	39
3.3.1 CalTempFromBias.....	39
3.3.2 CALNICA	41
3.3.3 Runcalsaa.....	54
3.4 Mosaicing/Drizzling.....	56
3.4.1 MultiDrizzle	56
3.4.2 Calnicb.....	56
3.5 Recalibration	62
3.5.1 Why Recalibrate?	62
3.5.2 Recalibrating the Data	63
3.6 Calibration Goals and Plans.....	67
3.6.1 Calibration Accuracies.....	67
3.6.2 Monitoring Programs	67
3.6.3 Special/Legacy Programs.....	69
3.6.4 SMOV Carry-over programs.....	69
3.6.5 Calibration in Previous Cycles.....	69
3.6.6 Special Calibrations	69

Chapter 4: Anomalies and Error

Sources	71
4.1 NICMOS Problems Checklist.....	71
4.2 NICMOS Dark Current and Bias	73
4.2.1 Dark Current	74
4.2.2 Bias, Shading, and “Pedestal”	77
4.2.3 Dark Reference Files	81
4.2.4 Cures: How To Get Rid of What's Left.....	85
4.3 Bars	91
4.4 Detector Nonlinearity Issues	93
4.4.1 Nonlinearity Calibrations.....	93
4.4.2 Non-Zero zeroth Read Correction for Bright Sources.....	94
4.4.3 Uncorrected Saturation.....	95
4.5 Count Rate Non-Linearity.....	96
4.6 Flat Fielding	98
4.6.1 Characteristics of NICMOS Flat Fields	98
4.6.2 Temperature-dependent Flat Fields	99
4.6.3 Color Dependence of Flat Fields	100

4.7 Pixel Defects and Bad Imaging Regions	101
4.7.1 Hot Pixels, Cold Pixels, and Grot.....	101
4.7.2 Erratic Middle Column/Row	103
4.7.3 Coronagraphic Hole.....	103
4.7.4 Vignetting.....	104
4.8 Effects of Overexposure	105
4.8.1 Photon Persistence.....	105
4.8.2 Cosmic Ray Persistence.....	106
4.8.3 Bright Earth Persistence (BEP)	109
4.8.4 Amplifier Ringing (The “Mr. Staypuft” Anomaly)	110
4.8.5 Optical Ghost Images	112
4.9 Cosmic Rays of Unusual Size.....	113
4.10 Scattered Earthlight.....	115

Chapter 5: Data Analysis

5.1 STSDAS Software	119
5.2 Photometric Calibrations	124
5.2.1 Units for NICMOS Photometry.....	124
5.2.2 Fluxes and Magnitude Zeropoints	124
5.2.3 Photometric Corrections	128
5.2.4 Absolute Photometry for Emission Line Filters.....	135
5.2.5 Absolute Spectrophotometry with NICMOS Grisms.....	136
5.3 Astrometry, Pixel scales, and Geometric Distortion	137
5.3.1 Pixel Scales	137
5.3.2 Geometric Distortion	138
5.3.3 Drizzling	140
5.3.4 Absolute Astrometry	141
5.4 PSF Subtraction	141
5.4.1 Impact of Instrumental Effects on PSF Subtraction	143
5.5 Coronagraphic Reductions	148
5.5.1 Data Products and File Structures.....	148
5.5.2 Coronagraphic Acquisitions.....	148
5.5.3 Positions of the Hole and Target	151
5.5.4 Recalibrating Coronagraphic Images	154
5.5.5 Reducing and Co-adding Coronagraphic Images...	157

5.6 Analysis of Polarization Images.....	162
5.6.1 Introduction	162
5.6.2 Theory.....	163
5.6.3 A Useful Script for Polarization Analysis.....	166
5.7 Grism Data Reduction.....	167
5.7.1 Extraction Software.....	168
5.7.2 Processing.....	169
Index	173

List of Figures

Figure 2.1: Data Format for ACCUM and BRIGHTOBJ Modes.....	14
Figure 2.2: MULTIACCUM Mode Data Format	14
Figure 3.1: Processing Flow for OTFR	36
Figure 3.2: Temperature for Individual Dark Images	40
Figure 3.3: Partial NICMOS Header	42
Figure 3.4: Calnica Processing Flow for a MULTIACCUM Observation	43
Figure 4.1: Dark Current Comparison Between Cycle 7 and Cycle 11.	75
Figure 4.2: Amplifier glow images for NICMOS cameras 1, 2 and 3.	77
Figure 4.3: Examples of shading for NICMOS cameras 1, 2 and 3	78
Figure 4.4: Data affected by variable quadrant bia.....	80
Figure 4.5: Bias jumps or “bands” in a NICMOS image.	81
Figure 4.6: NIC2 0.001024 BRIGHTOBJ mode exposure of HD10700	84
Figure 4.7: Bars in a NICMOS Camera 1 Image.	93
Figure 4.8: Figure 4.8: Graph of non-linearity by camera, top line NIC1, middle line NIC2, and bottom line NIC3	96
Figure 4.9: Flat-field responses for NIC1, NIC2 and NIC3.	99
Figure 4.10: Persistence induced by an exposure of a bright star.	106
Figure 4.11: Cosmic Ray Persistence in Three Dithered NIC2 MIF1024 Images.	107
Figure 4.12: NIC2 Persistence Images.....	110
Figure 4.13: The Mr. Staypuft Anomaly.	111
Figure 4.14: Optical ghosts in NIC1 polarizers.....	112

Figure 4.15: A “Monster Cosmic Ray” Hit in a NICMOS Image.	114
Figure 4.16: Plot of median counts vs. time for readouts from a NICMOS image.	116
Figure 4.17: Scattered light with difference.	116
Figure 5.1: Inverse sensitivity as function of temperature	129
Figure 5.2: Temperature dependent sensitivity as function of wavelength	130
Figure 5.3: Estimating Absolute Flux Variation.....	136
Figure 5.4: NIC1 Image with PSF Radial Profile	142
Figure 5.5: NIC2 Image with Radial Profile	143
Figure 5.6: Effect of cold mask wiggling on PSF subtraction in broad band and narrow band filters.	145
Figure 5.7: Illustration of PSF color dependence in different filters.	146
Figure 5.8: Effect of PSF color dependence on PSF subtraction in different filters.	147
Figure 5.9: Coronagraphic image, F110W filter.	159
Figure 5.10: PSF Subtraction.	161
Figure 5.11: PSF Subtraction.	161

List of Tables

Table 2.1: NICMOS File Name Suffixes	10
Table 2.2: NICMOS Science Data File Contents.....	13
Table 2.3: NICMOS Data Flag Values	15
Table 2.4: Science Data File Primary Header Keywords	20
Table 2.5: Image Extension Header Keywords in Science Data Files	26
Table 2.6: NICMOS Primary Header Keywords in the Support Files	27
Table 2.7: Some Useful NICMOS Extension Header Keywords in the Support Files	27
Table 2.8: NICMOS and NCS Telemetry Mnemonics	27
Table 2.9: Observation Information in iminfo Listing	28
Table 2.10: NICMOS-Specific Information in iminfo Listing.....	29
Table 3.1: Columns of the Association Table (input to calnicb)....	57
Table 3.2: Additional Columns of the Output Association Table ...	58
Table 3.3: Keywords Common to all Datasets in an Association	59
Table 3.4: Dataset-specific Keywords	59
Table 3.5: NICMOS CYCLE 17 Calibration Plan.....	68
Table 4.1: NICMOS Cosmetics (Cycle 11 and beyond, for masks produced in March 2009).....	102
Table 5.1: List of Stars for Photometric Transformations	135
Table 5.2: NICMOS Plate Scales at Detector Center (i.e. pixel 128, 128).....	138
Table 5.3: NICMOS Geometric Distortion Coefficients.....	139
Table 5.4: Beta Angles for all Three NICMOS Cameras	140

Table 5.5: Effect of focus variation, cold mask wiggling, and PSF color dependence on PSF subtraction.	144
Table 5.6: NICMOS ACQ Data Image Extensions	150
Table 5.7: NIC1 & NIC2 Polarizer Properties	164
Table 5.8: NIC1 & NIC2 Polarizer Properties for Cycle 11 and Beyond.....	165

Preface

How to Use this Handbook

This handbook is designed to help you manipulate, process and analyze data from the Near-Infrared Camera and MultiObject Spectrometer (NICMOS) on board the Hubble Space Telescope (*HST*). This is presented as an independent and self-contained document. Users who wish to find more general information about details of acquiring *HST* data from archive, their file formats, and general purpose software for displaying and processing these data, are referred to a companion volume, the "[HST Data Handbook](#)".

The current edition of the NICMOS Data Handbook has been written after servicing mission 3b (SM3b) and the installation of the NICMOS Cooling System (NCS). Therefore, where appropriate, details are given about the instrument performance in both pre- and post- NCS cycles. After the NCS installation (Cycles 11 and beyond), NICMOS had been operating at a warmer temperature ($77.15 \pm K$), leading to differences in calibration compared to Cycles 7/7N, as many of the instrument properties are temperature sensitive (e.g., dark current, bias behavior, quantum efficiency and hence, photometric calibration). NICMOS has been in the safe mode since September 2008 and NCS/NCS restart attempt has been deferred until after Servicing Mission 4. However, this handbook contains up-to-date information (as of March 2009), about photometric calibrations, bias-derived temperature, temperature dependent reference files, dark current and polarimetry. This handbook provides comprehensive information for treatment of the NICMOS data obtained during Cycles 7/7N, 11 and beyond. For updated information, readers are advised to consult the NICMOS Web pages on the Space Telescope Science Institute Web site for the latest information regarding NICMOS performance and calibration.

Typographic Conventions

To help you understand the material in the *NICMOS Data Handbook*, we will use a few consistent typographic conventions.

Visual Cues

The following typographic cues are used:

- **bold** words identify an **STSDAS**, **IRAF**, or **PyRAF** task or package name.
- typewriter-like words identify a file name, system command, or response that is typed or displayed as shown.
- *italic* type indicates a new term, an important point, or a mathematical variable, or a task parameter.
- SMALL CAPS identifies a header keyword.
- ALL CAPS identifies a table column.

Comments

Occasional side comments point out three types of information, each identified by an icon in the left margin.



Warning: *You could corrupt data, produce incorrect results, or create some other kind of severe problem.*



Heads Up: *Here is something that is often done incorrectly or that is not obvious.*



Tip: *No problems...just another way to do something or a suggestion that might make your life easier.*

Instrument Overview

In this chapter. . .

1.1 Instrument Overview / 1
1.2 Detector Readout Modes / 4

1.1 Instrument Overview

NICMOS was built by Ball Aerospace Corporation for the University of Arizona, under the direction of Rodger I. Thompson, the Principal Investigator. A basic description of the instrument and its on-orbit performance through the Servicing Mission Orbital Verification program is provided by Thompson et. al (1998).¹ We encourage all NICMOS users to reference this paper and to review the related papers in the special issue of *ApJ Letters* which describe the Early Release Observations and demonstrate the scientific capabilities of NICMOS. The *NICMOS Instrument Handbook* and the NICMOS Web pages at:

<http://www.stsci.edu/hst/nicmos>

are also valuable sources of information for the NICMOS user, particularly concerning technical details of the instrument, as well as a history of its performance throughout its lifetime. The NICMOS edition of the *Space Telescope Analysis Newsletter (STAN)*, which is periodically distributed by e-mail², provides regular notices and updates to information about NICMOS and NICMOS data reduction. Back issues of the NICMOS STAN are archived at the STScI [NICMOS Web](#) site.

1. Thompson, R.I., M. Rieke, G. Schneider, D.C. Hines, and M.R. Corbin, 1998, *ApJL*, 492, L95.

2. To subscribe to the *STAN*, send a message to majordomo@stsci.edu with the Subject: line blank and “subscribe nicmos_news” in the body).

The first phase of life for NICMOS took place during *HST* Cycle 7, with a special, supplemental call for proposals issued as Cycle 7N. Its cryogens were exhausted in January 1999, and the instrument was deactivated and subsequently decommissioned. The installation of NICMOS Cooling System (NCS) during Servicing Mission 3B in March 2002, brought NICMOS back down to cryogenic temperatures, and returned it to regular service in Cycle 11.

In September 2008 the flight software for the spacecraft computer (NSSC-I) had to be updated in order to accommodate the new instruments to be installed during Servicing Mission 4. Since this computer manages the health and safety of all the on-board instruments, including NICMOS and the NICMOS Cooling System / NICMOS Cryo-cooler (NICMOS NCS/NCC), this involved shutting down the NCS/NCC as part of the procedure, on Sept. 10, 2008. After the NSSC-I update, the NCS was restarted but went into safe mode soon afterwards, before the cool down had completed. It safed few more times with telemetry suggesting presence of icy contaminants interfering with the circulator pump. There was no indication of any damage to the mechanical systems in the NCS/NCC or to NICMOS itself, for the brief amounts of time that the system was running during each restart attempt. The circulator was allowed to warm up over a period of few months, reaching temperatures sufficiently warm to enable any contaminants to thaw and be more easily removed once the circulator was restarted. NCS/NCC was restarted and cooling was successfully commenced. NCS safed again after a couple of restart attempts but this time the safing was caused by a low speed limit violation of the Turbo Alternator, which helps to maintain the proper flow rate of coolant. The HST Project thereafter decided to defer subsequent NICMOS Cooling System startup attempts until after Servicing Mission 4.

This edition of the NICMOS Data Handbook is based on experience with NICMOS data obtained in Cycles 7 and 7N, before NCS installation, and in Cycles 11 through 16, after NCS installation. However, the NICMOS data reduction described in this handbook is mainly intended for reduction of data obtained in Cycles 11 and beyond. Where appropriate, major differences after NCS installation are indicated, but when reducing Cycle 7 or 7N data, be sure to also consult version 5.0 of this Data Handbook.

NICMOS provides imaging capabilities in broad, medium, and narrow band filters, broad-band imaging polarimetry, coronagraphic imaging, and slitless grism spectroscopy in the wavelength range 0.8–2.5 μm . NICMOS is an axial instrument with three adjacent but not contiguous cameras,

designed to operate independently and simultaneously. Optical elements, integration times, and readout modes can be different for each. Each camera has a different magnification scale, and is equipped with a dedicated 256×256 HgCdTe Rockwell array. The approximate pixel sizes and fields of view are $0''.043$ and $11'' \times 11''$ for Camera 1 (referred to as NIC1), $0''.075$ and $19''.2 \times 19''.2$ for NIC2, and $0''.2$ and $51''.2 \times 51''.2$ for NIC3.

Each camera is provided with its own set of filters, mounted on three independent wheels. There are a total of 20 filter positions on each wheel, of which one is blank (i.e., a cold, opaque filter used in lieu of a dark slide). Three of the other positions are occupied by either polarizers or grisms. The remaining 16 positions of each filter wheel are occupied by broad, medium, and narrow band filters. The list of these filters is given in the *NICMOS Instrument Handbook*. The filters (including polarizers and grisms) cannot be crossed with each other, and are used as single optical elements.

NIC1 and NIC2 each contain three polarizers, whose principal axes of transmission are separated by approximately 120 degrees (for the exact polarizer orientations and other details, see Section 5.6 of this manual, and also Chapter 5 of the *NICMOS Instrument Handbook*). The spectral coverage is fixed for each camera. The polarizers cover the wavelength range $0.8\text{--}1.3\text{ }\mu\text{m}$ in NIC1, and $1.9\text{--}2.1\text{ }\mu\text{m}$ in NIC2. Observations in the three polarizers of each camera are used to derive the Stokes parameters of linearly polarized light.

The filter wheel of NIC3 contains three grisms which can be used to perform slitless spectroscopy in the wavelength range $0.8\text{--}2.5\text{ }\mu\text{m}$. The three grisms cover the range $0.8\text{--}1.2\text{ }\mu\text{m}$, $1.1\text{--}1.9\text{ }\mu\text{m}$, and $1.4\text{--}2.5\text{ }\mu\text{m}$, respectively.

In NIC2, a coronagraphic spot is imaged onto the focal plane and provides a circular occulted region $0''.3$ in radius (with a useful effective radius of $0''.4$). For coronagraphic imaging, an acquisition sequence is required at the beginning of the observation to center the target under the occulting spot.

Each 256×256 detector array is divided into four 128×128 quadrants, each of which is read out by an amplifier at the corner of the quadrant. There are four amplifiers in each camera. Unlike CCDs, infrared array pixels are read independently and problems like charge transfer efficiency or bleeding are not present.

1.2 Detector Readout Modes

NICMOS does not have a physical shutter mechanism, and exposures are obtained through a sequence of reset and read operations. In particular, a typical exposure will be the product of the following steps:

1. **Array reset:** the pixels are set to the bias level.
2. **Array read:** the charge in each pixel is measured and stored in the on-board computer's memory. This read is performed immediately after the reset, and contains the reference level for the exposure (*zeroth read*). In practice, the readout is performed 0.203 seconds after the reset, implying that it represents a finite, though very short, exposure. This readout is performed non-destructively; the charge in each pixel is left intact.
3. **Integration:** NICMOS integrates for the user-specified time.
4. **Array read:** the charge in each pixel is measured and stored in the on-board computer's memory. Again, the readout is non-destructive.

The beginning of an integration is marked by the zeroth read, which is always preceded by a reset. Since all readouts are non-destructive, i.e., do not change the value of the charge accumulated on the pixel, the last two steps of the sequence above can be repeated multiple times, and the last read of the sequence will be called the *final read*. The total integration time of an exposure is defined as the time between the final and the zeroth read of the first pixel in the array. The scientific image is given by the difference between the final and the zeroth readouts.

Four readout modes have been defined for NICMOS, exploiting the flexibility allowed by the non-destructive reads:

- MULTIACCUM
- ACCUM
- BRIGHTOBJ
- RAMP (not available in Cycle 11 and beyond).

Each mode is described in the following sections, with larger emphasis on MULTIACCUM, which is by far the most used and best calibrated mode. RAMP mode was never used for on-orbit science observations during Cycle 7, and is no longer available for use in Cycle 11 and beyond.

1.2.1 MULTIACCUM

In a MULTIACCUM (MULTIple ACCUMulate) exposure, the zeroth read is followed by several other non-destructive readouts during the course of a single integration. All of the readouts are stored in the on-board computer's memory and sent to the ground. Because the readouts are non-destructive, accumulated counts are built up from one readout to the next, with the last readout containing the accumulated counts from the entire integration time of the observation. In an exposure, the number of readouts after the zeroth and the temporal spacing between each read is selected by the user from a set of 16 pre-defined *sequences*. The sequence chosen by the user is stored in the value of the `SAMP_SEQ` keyword in the science data files. The user specifies the number of readouts through the `NSAMP` keyword during the Phase II proposal process. `NSAMP+1` (including the zeroth read) images will be returned to the ground. For NICMOS the maximum value of `NSAMP` is 25 in each sequence (for a total of 26 images returned to the ground).

MULTIACCUM gives information not only at the beginning and at the end of an exposure, but also at intermediate times. It is the mode of choice for the vast majority of astronomical observations, from objects with large dynamical range to deep field integrations. The intermediate reads can also be used to remove the effects of cosmic ray hits and of saturated pixels from the final processed image.



The images returned to the ground by the MULTIACCUM readout are raw detector readouts, since not even the bias level (the zeroth read) is subtracted. This operation is performed by the ground calibration pipeline.

1.2.2 ACCUM

ACCUM is a simplified version of MULTIACCUM: the zeroth read is followed by one read (the final readout) after an amount of time specified by the integration time. The difference between the final and the zeroth readouts is computed on-board, and the resulting image is sent to the ground. In this form, the ACCUM mode produces data very similar to the more familiar CCD images. A variation to this basic operation is available, which replaces the single initial and final readouts with multiple (initial and final) readouts. After the initial reset pass, n non-destructive reads of the detector immediately follow, as close together in time as allowed by the detector electronics. The average of the n values is stored as the initial value for each pixel. At the end of the integration, there are again n

non-destructive readouts with the final value for each pixel being the average of the n reads. The number n of initial and final reads is specified by the observer and is recorded in the value of the NREAD (number of reads) header keyword in the science data files. The returned image is the difference between the averaged final and initial values. The integration time is defined as the time between the first read of the first pixel in the initial n passes and the first read of the first pixel in the final n passes. The advantage of the multiple initial and final (MIF) readout method is that, in theory, the read noise associated with the initial and final reads should be reduced by a factor of \sqrt{n} , where n is the number of reads (see, e.g., Fowler and Gatley 1990, ApJ, 353, L33). In practice, actual noise reduction in NICMOS observations is generally rather less than \sqrt{n} for a variety of reasons, such as amplifier glow (see Section 4.2.1). Any NREAD value up to 25 can be used, but the only supported NREAD values are 1 and 9. The **calnica** software may be updated to support any NREAD value in further releases. See the NICMOS Web page for updates.

1.2.3 BRIGHTOBJ

The BRIGHTOBJ (BRIGHT OBJECT) mode provides a way to observe objects that would usually saturate the detector in less than the minimum available exposure time (which is the amount of time it takes to read out the array and is 0.203 seconds). In BRIGHTOBJ mode each individual pixel (per quadrant) is successively reset, read, integrated for a time requested by the observer, and read again, and then these steps are performed for the next pixel in the quadrant. The returned image contains the number of counts accumulated between the initial and final reads for each pixel (just like ACCUM mode). Since each quadrant contains 16,384 pixels, the total elapsed time to take an image in this mode is 16,384 times the requested exposure time for each pixel. BRIGHTOBJ is essentially an ACCUM mode exposure, but the readout timing is different.



BRIGHTOBJ mode was rarely used for on-orbit science observations and is essentially uncalibrated. Since Cycle 11, BRIGHTOBJ is an available observing mode for the special case of acquisition of very bright targets for coronagraphy, but this mode is not supported by STScI.

1.2.4 RAMP

RAMP mode was designed to use multiple non-destructive reads during the course of a single exposure much like MULTIACCUM, but only a single image is sent to the ground. In principle, RAMP mode could be used to obtain the benefits of a MULTIACCUM exposure without the large data volume. However the difficulty of implementing infallible algorithms for on-board processing made this mode impractical, and its use for on-orbit observations was discouraged in Cycles 7 and 7N. Indeed, almost no data were obtained in RAMP mode, and it has not been supported for NICMOS observing in Cycles 11 and beyond. We describe the mode here for historical reasons only, and it will not be considered otherwise in this *Handbook*.

In RAMP mode, the total integration time T is divided into n equal intervals $t = T / n$. Each readout is differenced (on-board) with the previous readout and used to compute a running mean of the number of counts (per sample interval) and an associated variance for each pixel. Large deviations from the running mean are used to detect saturation or a cosmic ray hit. At the end of the exposure, the data sent to the ground comprise a mean countrate image, plus the variance and the number of valid samples used to compute each pixel value. The effective exposure time for the returned image is the sample interval t .



Almost no data were obtained in RAMP mode during Cycles 7 and 7N, and it has not been supported for NICMOS observing in Cycles 11 and beyond. The reduction and analysis of RAMP mode data will not be discussed further in this Handbook.

Data Structures

In this chapter. . .

2.1 NICMOS Data Files / 9
2.2 Header Keywords / 19
2.3 Working with NICMOS Files / 28
2.4 From the Phase II Proposal to Your Data / 31
2.5 Paper Products / 33

2.1 NICMOS Data Files

STScI automatically processes and calibrates all NICMOS data and archives the data files resulting from pipeline processing in FITS format. If you have retrieved NICMOS files from the Archive, you will notice that their names look like this:

```
n3w2a1wqm_cal.fits
```

The first part of the file name (`n3w2a1wqm`) is the *rootname*, identifying the dataset to which the file belongs, the second (`cal`) is the *suffix*, identifying the type of data the file contains, and the third (`fits`) indicates that this is a FITS format file. Chapter 2 of the "[HST Data Handbook](#)" shows how to access the data contained in NICMOS FITS files, while Appendix B of the "[HST Data Handbook](#)" explains how to decipher the rootnames of these files and explains why some of them are grouped into data *associations*. This section describes the files that constitute a NICMOS dataset.

2.1.1 File Name Suffixes

Each file in a NICMOS dataset has a three-character suffix that uniquely identifies the file contents. The file name suffixes for NICMOS and the corresponding file contents are summarized below. Table 2.1 lists all of the files that the pipeline can produce. For some observing strategies not all of the processing steps are performed and only a subset of these files will be produced by the pipeline.

Table 2.1: NICMOS File Name Suffixes

Extension	Image Contents
ipppssoot_asc	Post-calibration association table (produced by calnicb)
ipppssoot_asn	Association table (for dithered pattern observations)
ipppssoot_cal	Calibrated science data file
ipppssoot_clb	Calibrated background data file (for ACCUM mode only)
ipppssoot_clf	Calibrated flat-field data file (for ACCUM mode only)
ipppssoot_epc	Temperature telemetry table
ipppssoot_ima	Intermediate MULTIACCUM science data file
ipppssoot_mos	Combined image produced by calnicb
ipppssoot_raw	Raw science data file
ipppssoot_rwb	Raw background data file (for ACCUM mode only)
ipppssoot_rwf	Raw flat-field data file (for ACCUM mode only)
ipppssoot_spb	Background SHP and UDL information (for ACCUM mode only)
ipppssoot_spf	Flat-field SHP and UDL information
ipppssoot_spt	Target SHP and UDL information
ipppssoot_trl	OPUS processing trailer file
ipppssoot_pdq	OPUS Processing Data Quality file (discontinued May 9, 2002)

- Raw Data Files

- *Raw Science File* (**_raw**):

This FITS file contains the raw image data received from the spacecraft. One file per exposure is created (a MULTIACCUM exposure is considered a single exposure irrespective of the number of samples specified).

- *Support File* (**_spt**):

This FITS file contains supporting information about the observation, the spacecraft telemetry and engineering data from the instrument that was recorded at the time of the observation, including detector temperature measurements.

- *Association Table* (`_asn`):
This file is a FITS binary table that contains the list of datasets making up an association.
- Calibrated Data Files
 - *Calibrated Science File* (`_cal`):
This FITS file contains the calibrated science data for an *individual dataset*, and is produced by the pipeline calibration task **calnica** (see Chapter 3). The input to **calnica** are the `_raw` images. For a MULTIACCUM exposure, this file contains a single science image formed by combining the data from all samples.
 - *Intermediate Multiaccum Science File* (`_ima`):
This FITS file is also produced by the pipeline task **calnica** and contains the calibrated science data for all samples of a MULTIACCUM dataset before the process of combining the individual readouts into a single image has occurred. This file is only produced for MULTIACCUM observations.
 - *Mosaic Files* (`_mos`):
These FITS files contain the composite target and, for chopped pattern sequences, background region images constructed by the pipeline task **calnicb** for an associated set of observations (see Chapter 3). The input to **calnicb** are the calibrated `_cal` images from **calnica** and the `_asn` association table. Target images are co-added and background-subtracted. The value of the last character of the rootname is 0 for targets, and 1 to 8 for background images. These files are only produced for an associated set of observations.
 - *Post-calibration Association Table* (`_asc`):
This table is produced by the pipeline calibration task **calnicb**, and is the same as the association table `_asn`, with the addition of new columns which report the offsets between different images of the mosaic or chop pattern as calculated by **calnicb**, and the background levels computed for each image. This file is only produced for an associated set of observations.
 - *Trailer File* (`_trl`):
This FITS ASCII table contains a log of the pipeline calibration processing that was performed on individual datasets and mosaic products.

- *Processing Data Quality File* (`_pdq`):
This FITS ASCII table provides quality information on the observation, mostly on pointing and guide star lock. Possible problems encountered, e.g., a loss of guide star lock or a guide star acquisition failure, are reported here.
- *Temperature Telemetry Table* (`_epc`):
This FITS binary table is produced by the Engineering Data Processing System (EDPS) as an aid for use in calibration and temperature monitoring. Nine NICMOS Cooling System (NCS) mnemonics and five temperature sensors are bundled together into an **STSDAS** FITS table. (Available after OPUS 15.2)

2.1.2 Science Data Files

The `*_raw.fits`, `*_cal.fits`, `*_ima.fits`, and `*_mos.fits` files are all defined as *science data files*, as they contain the images of interest for scientific analysis.

File Contents and Organization

The data for an individual NICMOS science readout consist of five arrays, each stored as a separate image extension in the FITS file. The five data arrays represent:

- The science (SCI) image from the detector.
- An error (ERR) array containing an estimate of the statistical uncertainties (corresponding to 1σ uncertainties) of the science data.
- An array of bit-encoded data quality (DQ) flags representing known status or problem conditions of the science data.
- An array containing the number of data samples (SAMP) that were used to compute each science image pixel value.
- An array containing the effective integration time (TIME) for each science image pixel.

A grouping of the five data arrays for one science image is known as an *image set* or *imset*.

A science data file can contain one or more imsets. For example, an individual NICMOS exposure obtained with the ACCUM mode will generate a `*_raw.fits` file with one imset; an individual MULTIACCUM exposure with n readouts will generate a `*_raw.fits` file (and, after calibration, an `*_ima.fits` file) containing $n + 1$ imsets, including the zeroth readout. The `*_cal.fits` and `*_mos.fits` files always contain one imset.



The imsets of a MULTIACCUM exposure are stored in files from last to first. The result of the longest integration time (the last readout performed on-board) occurs first in the file (first imset), the readout before the last is the second imset, and so on; the zeroth readout is the last imset.

Although the five science, error, data quality, samples, and integration time arrays associated with each imset are stored in a single file, they are kept separate as five individual FITS image *extensions* within the file. The order of the images in the FITS files is listed in Table 2.2 and shown graphically in Figure 2.1 and Figure 2.2. The examples given in Table 2.2 and Figure 2.2 refer to a MULTIACCUM image (multiple imsets), while Figure 2.1 refers to ACCUM and BRIGHTOBJ images (one imset, namely extensions 1 through 5). Each extension comes with its own header, and each FITS file contains, in addition, a *global* or *primary header* (primary header-data unit or HDU).

The only contents of the primary HDU are header keywords. There are no image data in the primary HDU. The keywords in the primary header are termed *global keywords* because they apply to the data in all of the file extensions. The organization and location of header keywords is explained in detail later in the chapter.

Table 2.2: NICMOS Science Data File Contents

Header-Data Unit	Extension Name	imset	Contents	Data Type
Primary (Extension 0)	(N/A)	(N/A)	Global keywords; no data.	(N/A)
Extension 1	SCI	1	Science image	raw: 16-bit int; calibrated: float
Extension 2	ERR	1	Error (sigma) image	float
Extension 3	DQ	1	Data Quality image	16-bit int
Extension 4	SAMP	1	Number of Samples image	16-bit int
Extension 5	TIME	1	Integration Time image	float
Extension 6	SCI	2	Science image	raw: 16-bit int; calibrated: float
Extension 7	ERR	2	Error (sigma) image	float
Extension 8	DQ	2	Data Quality image	16-bit int
Extension 9	SAMP	2	Number of Samples image	16-bit int
Extension 10	TIME	2	Integration Time image	float

Figure 2.1: Data Format for ACCUM and BRIGHTOBJ Modes


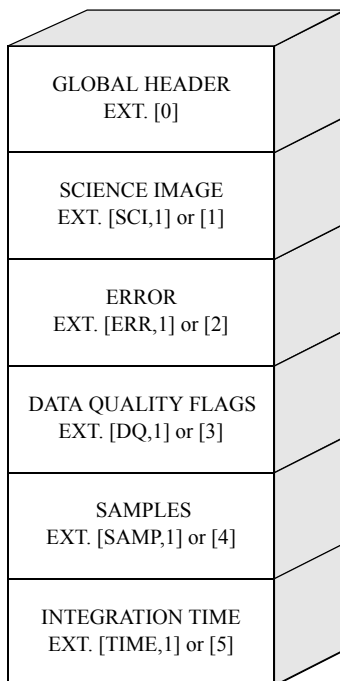


Figure 2.2: MULTIACCUM Mode Data Format

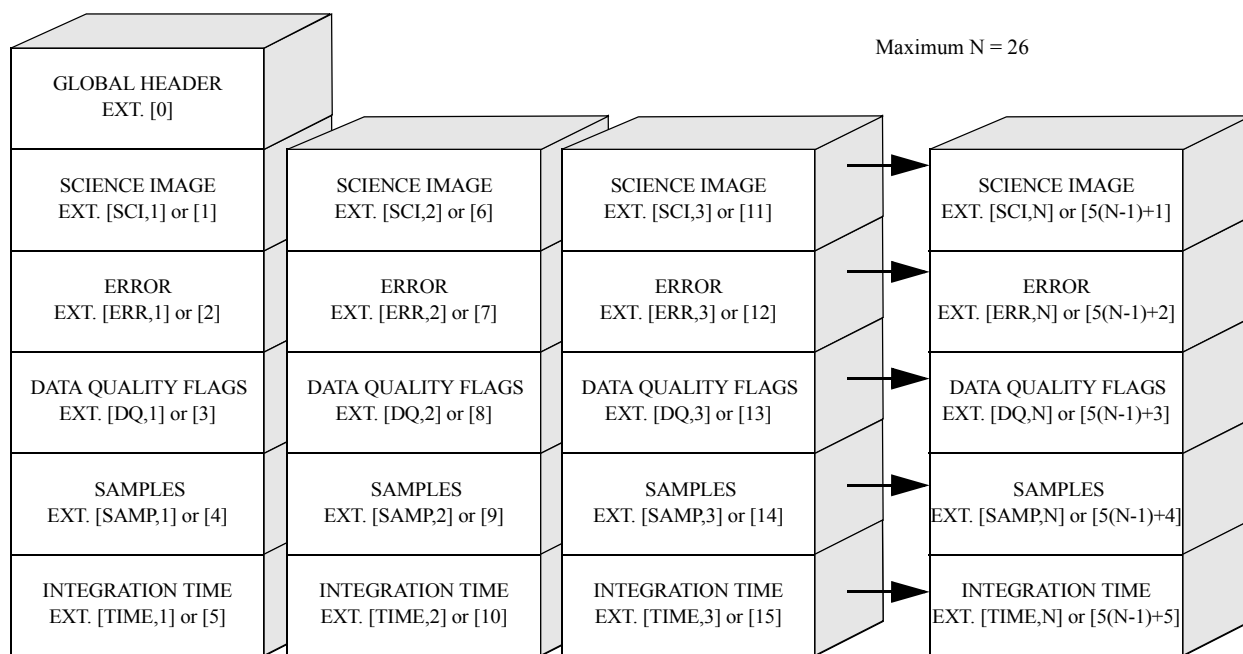

The following sections explain the contents and origin of each of the five image arrays in each imset in more detail.

Science Image

This image contains the data from the detector readout. In ACCUM and BRIGHTOBJ modes the image received from the instrument is the result of subtracting the initial from the final readouts of the exposure. In MULTIACCUM mode the images received are the raw (unsubtracted) data corresponding to each detector readout. In raw datasets the science array is an integer (16-bit) image in units of DN_s (counts). In calibrated datasets it is a floating-point image in units of DN_s per second (count rates).

Error Image

The error image is a floating-point array containing an estimate of the statistical uncertainty associated with each corresponding science image pixel. This image is computed in the ground calibration pipeline task **calnica** as a combination of detector read noise and Poisson noise in the accumulated science image counts (see Chapter 3) and corresponds to 1σ uncertainties. For calibrated MULTIACCUM images (i.e., *_cal.fits files), the values of the error array are computed uncertainties in the count rates derived from the linear fit to counts vs. exposure time from the intermediate readouts.

Data Quality Image

This integer (unsigned 16-bit) array contains bit-encoded data quality flags indicating various status and problem conditions associated with corresponding pixels in the science image. Because the flag values are bit-encoded, a total of 16 simultaneous conditions can be associated with each pixel. Table 2.3 lists the flag values and their meanings.

Table 2.3: NICMOS Data Flag Values

Flag Value	Bit Setting ¹	Flag Meaning
0	0000 0000 0000 0000	No known problems
1	0000 0000 0000 0001	Reed-Solomon decoding error in telemetry
2	0000 0000 0000 0010	Poor or uncertain Linearity correction
4	0000 0000 0000 0100	Poor or uncertain Dark correction
8	0000 0000 0000 1000	Poor or uncertain Flat-Field correction
16	0000 0000 0001 0000	Pixel affected by “grot” on the detector
32	0000 0000 0010 0000	Defective (hot or cold) pixel
64	0000 0000 0100 0000	Saturated pixel
128	0000 0000 1000 0000	Missing data in telemetry
256	0000 0001 0000 0000	Bad pixel determined by calibration
512	0000 0010 0000 0000	Pixel contains Cosmic Ray
1024	0000 0100 0000 0000	Pixel contains source (see Section 3.4)

Flag Value	Bit Setting ¹	Flag Meaning
2048	0000 1000 0000 0000	Pixel has signal in 0th read (see Section 3.3)
4096	0001 0000 0000 0000	Cosmic ray detected by MultiDrizzle
8192	0010 0000 0000 0000	User flag
16384	0100 0000 0000 0000	Curvature in detector response

1. Most significant bit is at left.

Number of Samples Image

The SAMP image is an integer (16-bit) array containing the total number of data samples that were used to compute the corresponding pixel values in the science image. For ACCUM and BRIGHTOBJ modes, the number of samples contributing to each pixel always has a value of 1 in the raw data file. For MULTIACCUM mode the sample values in the raw and intermediate data files are set to the number of readouts that contributed to the corresponding science image.



Because the number of samples in the raw images for MULTIACCUM, ACCUM and BRIGHTOBJ modes is the same value for all pixels of an imset, the image array is usually not created (to save on data volume), and the value of the sample is stored in the header keyword PIXVALUE in the SAMP image extension (see Table 2.5 below).

In MULTIACCUM calibrated data files (*_cal.fits) the SAMP array contains the total number of valid samples used to compute the final science image pixel value, obtained by combining the data from all the readouts and rejecting cosmic ray hits and saturated pixels. In this case the sample array may have different values at different pixel locations (less than or equal to the total number of samples in the MULTIACCUM sequence), depending on how many valid samples there are at each location.

In the mosaic images (*_mos.fits), the data in the SAMP array indicate the number of samples that were used from overlapping images to compute the final science image pixel value.

Integration Time Image

The TIME image is a floating-point array containing the effective integration time associated with each corresponding science image pixel value. These data are always computed in the ground calibration pipeline for recording in the raw data file.



For ACCUM and BRIGHTOBJ mode observations, each pixel has the same time value. For MULTIACCUM observations each pixel for a given readout has the same time value in the raw and intermediate data. In these cases, to save on data volume, the image array is not created and the value of the time is stored in the header keyword PIX-VALUE in the TIME image extension (see Table 2.5).

In MULTIACCUM calibrated data files (`*_cal.fits`) the TIME array contains the combined exposure time of all the readouts that were used to compute the final science image pixel value, after rejection of cosmic ray and saturated pixels from the intermediate data. As in the case of the SAMP array, the TIME array can have different values at different pixel locations, depending on how many valid samples compose the final science image in each pixel.

In mosaic images (`*_mos.fits`), the TIME array values indicate the total effective exposure time for all the data from overlapping images that were used to compute the final science image pixel values.

2.1.3 Auxiliary Data Files

The `*_spt.fits`, `*_trl.fits`, `*_pdq.fits`, `*_asn.fits`, and the `*_asc.fits` files are termed *auxiliary data files*. They contain supporting information on the observation, such as spacecraft telemetry and engineering data, assessment of the quality of the observation, calibration information, and information on the associations present in the observations.

Association Tables

The *association tables*, `*_asn.fits` and `*_asc.fits`, are FITS binary tables which are created when a particular observation generates an association of datasets (see the discussion of “Associations” in Appendix B of the ["HST Data Handbook"](#)). In particular, the `*_asn.fits` table is generated by OPUS¹, and contains the list of datasets which make up the association (e.g., from a dither or chop pattern). The `*_asn.fits` tables are the inputs to the pipeline **calnicb**, which creates the mosaiced or background subtracted images (`*_mos.fits` files) from the input datasets. All the datasets must have been processed through the basic pipeline data reduction (**calnica**) before being processed through **calnicb**. In addition to the output science image(s), **calnicb** produces another association table (`*_asc.fits`), which has the same content as the

1. Observation Support & Post Observation Data Processing Unified Systems

`*_asn.fits` table, along with additional information on the offsets used by the pipeline for reconstructing the science image and background values computed for each image. For mosaics (dither patterns), there is only one final image produced, with file name `*0_mos.fits`. For chop patterns, in addition to the background-subtracted image of the target (`*0_mos.fits`), an image for each background position is produced; the file names of these background images are `*1_mos.fits`, `*2_mos.fits`, ..., `*8_mos.fits` (a maximum of eight independent background positions is obtainable with the NICMOS patterns; see the *NICMOS Instrument Handbook* for details).

Support File

The support files, `*_spt.fits`, contain information about the observation and engineering data from the instrument and spacecraft that was recorded at the time of the observation. A support file can have multiple FITS image extensions within the same file; in the case of a MULTIACCUM observation there will be one extension for each readout (i.e., each imset) in the science data file. Each extension in the support file holds an integer (16-bit) image containing the data which populates the `*_spt.fits` header keyword values.

Trailer File

The trailer files, `*_trl.fits`, contain information on the calibration steps executed by the pipelines and diagnostics issued during the calibration. There is one `*_trl.fits` file produced for each dataset, and, in the case of associations, one `*_trl` file for each NICMOS product (i.e., each `*_mos.fits` file).

Processing Data Quality File

The processing data quality files, `*_pdq.fits`, contain general information summarizing the observation, a data quality assessment section, and a summary on the pointing and guide star lock. They state whether problems were encountered during the observations, and, in case they were, describe the nature of the problem. There is one `*_pdq.fits` file produced for each dataset, and, in case of associations, one `*_pdq` file for each NICMOS product (i.e., each `*_mos.fits` file).

Temperature Table

The temperature tables, `*_epc.fits`, contain a set of 14 mnemonics (sensors) extracted from the engineering telemetry. The time range of the tables are over the duration of the corresponding observations. The selected sensor used to monitor the temperature of the NICMOS detectors is NDWTMP11, the temperature at the NIC1 mounting cup. A listing of the individual table names and their location within the FITS table can be obtained by using the IRAF/STSDAS task `catfits`. (See [NICMOS ISR 2003-008](#) for more details.) Mnemonics in the temperature table `*_epc.fits`,

report temperature information within the NCS and five temperature sensors within the NICMOS dewar. Table 2.8 presents a listing of the 14 NCS and NICMOS telemetry temperature sensors.

2.2 Header Keywords

Both the primary header and the headers of each image extension in a science data file contain *keywords*. The keywords store a wide range of information about the observations themselves (e.g., observing mode, integration time, filters or grisms used), the processing of the data by the OPUS pipeline (e.g., calibration steps performed and reference files used), and the properties of the data themselves (e.g., number of image extensions, dimensions and data type of each image, coordinate system information, flux units, and image statistics).

The primary header carries global keywords which are applicable to all extensions. The extension headers carry extension-specific keywords, which contain information relevant to the image in a particular extension. For example, observation parameters, calibration switches and reference file names are contained in the primary header. Exposure time and World Coordinate System information, on the other hand, are contained in the header of each image extension because this information could vary from one set of extensions to another.

Table 2.4 below lists most of the keywords in the primary header of the *science data files*. The entries in this table are appropriate for data retrieved in 2009 from the *HST* Archive via on-the-fly reprocessing (OTFR - see Chapter 3). Some header keywords in older NICMOS data may be different. In particular, the observing pattern keywords have been changed for Cycle 11, and the dictionary below describes the new keyword format. The post-SAA dark keywords have been in use since Cycle 11. For data taken in Cycle 7 and 7N, these keywords are not populated. Since April 2007, the SAAClean task has been incorporated into the OTFR to clean SAA persistence from science observations. The related keywords can be found in the **SAACLEAN** and **RUNCALSAA** sections of Table 2.4. Keywords associated with the bright earth persistence and the bias-derived temperature were added to the OTFR in march 2008 in OPUS version 2008.1. The STScI Data Processing Team maintains a complete [HST FITS header keyword dictionary](#) with descriptions of the keywords used by NICMOS and other *HST* instruments.

Table 2.4: Science Data File Primary Header Keywords

Keyword Name	Meaning
Image Keywords	
NEXTEND	Number of extensions in the file (up to 130 for MULTIACCUM).
DATE	Date on which the file was generated
FILENAME	Name of the file
FILETYPE	Type of data: SCI - Science Data File; SPT - Support File; ASN_TABLE - Association Table
TELESCOP	HST
INSTRUME	Instrument used (NICMOS)
EQUINOX	Equinox of the celestial coordinate system (J2000.0 for HST observations)
Data Description Keywords	
ROOTNAME	Rootname (IPPPSSOOT) of the dataset
IMAGETYP	Image type: EXT = external image; FLAT = flatfield image; DARK = dark image
PRIMESI	Primary Instrument used for the observation
Target Information	
TARGNAME	Proposer's target name
RA_TARG	Right Ascension of the target (degrees, J2000)
DEC_TARG	Declination of the target (degrees, J2000)
ECL_LONG	Ecliptic longitude of the target (deg) (J2000)
ECL_LAT	Ecliptic latitude of the target (deg) (J2000)
GAL_LONG	Galactic longitude of the target (deg) (J2000)
GAL_LAT	Galactic latitude of the target (deg) (J2000)
Other Coordinate System Information	
APER_REF	Aperture used for reference position
ELON_REF	Ecliptic longitude at reference position (deg)
ELAT_REF	Ecliptic latitude at reference position (deg)
GLON_REF	Galactic longitude at reference position (deg)
GLAT_REF	Galactic latitude at reference position (deg)
Proposal Information	
PROPOSID	Proposal's identification number
LINENUM	Exposure's logsheet line number, from the Phase 2 proposal
PR_INV_L	Principle investigator last name
PR_INV_F	Principle investigator first name
PR_INV_M	Principle investigator middle initial
Exposure Information	
ORIENTAT	Position angle of the image y axis (degrees East of North)
SUNANGLE	Angle between sun and V1 axis
MOONANGL	Angle between moon and V1 axis
SUN_ALT	Altitude of the sun above earth's limb
FGSLOCK	Commanded FGS lock (FINE, COARSE, GYROS, UNKNOWN)
GYROMODE	Number of gyros scheduled for observation
REFFRAME	guide star catalog version
DATE-OBS	UT date of start of the observation (dd/mm/yy or yyyy-mm-dd)
TIME-OBS	UT time of start of the observation (hh:mm:ss)
EXPSTART	Exposure start time (Modified Julian Date)

Table 2.4: Science Data File Primary Header Keywords

Keyword Name	Meaning
EXPEND	Exposure end time (Modified Julian Date)
EXPTIME	Total integration time (sec)
EXPFLAG	Exposure interruption indicator (e.g., NORMAL)
<i>Instrument Configuration Information</i>	
CAMERA	NICMOS camera used in the observation (1, 2, or 3)
PRIMECAM	NICMOS Prime Camera during the observation (for internal parallels)
FOCUS	In-focus camera for this observation
APERTURE	Aperture used in the observation (NICi, NICi-FIX, NIC2-CORON)
OBSMODE	Observing mode (MULTIACCUM, ACCUM,...)
FILTER	Filter or grism used
NUMITER	Number of iterations of the exposure
NREAD	Number of ACCUM initial and final readouts
NSAMP	Number of MULTIACCUM or RAMP samples
SAMP_SEQ	MULTIACCUM exposure time sequence name
FOMXPOS	X offset of the Camera FOV using NICMOS FOM (arcsec)
FOMYPOS	Y offset of the Camera FOV using NICMOS FOM (arcsec)
NFXTILTP	FOM X-tilt position (arcsec)
NFYTILTP	FOM Y-tilt position (arcsec)
NPXTILTP	PAM X-tilt position (arcsec)
NPYTILTP	PAM Y-tilt position (arcsec)
NPFOCUSP	PAM focus position (mm)
TIMEPATT	Timing pattern identifier for readout
READOUT	Detector array readout rate (FAST, SLOW)
SAMPZERO	Sample time of MULTIACCUM zeroth read (sec)
HCLKRATE	Horizontal clock rate (microseconds)
VIDEO_BW	Readout video bandwidth (kHz)
ADCGAIN	Analog-digital conversion gain (electrons/DN)
<i>Photometry Keywords</i>	
PHOTMODE	Combination of <INSTRUMENT>+<CAMERA>+<FILTER>
PHOTFLAM	Inverse sensitivity (erg/cm ² /angstrom/DN)
PHOTFNU	Inverse sensitivity (Jy*sec/DN)
PHOTZPT	ST magnitude system zero point
ZPSCALE	Temp dependent photometric zero-point scale factor
PHOTFERR	Relative error:temp dependent photometric zero-point
PHOTPLAM	Pivot wavelength of the photmode (Angstrom)
PHOTBW	Root Mean Square bandwidth of the photmode (Angstrom)
<i>Bias-Derived Temperature Information</i>	
TFBDATE	Date that CalTempFromBias was run
TFBERR	Error (deg K) for temperature derived from bias
TFBMETH	CalTempFromBias algorithm type used
TFBTEMP	Temperature (deg K) derived from bias
TFBVER	Version of CalTempFromBias run
<i>Bias-Derived Temperature Calibration Switches</i>	
TFBCALC	CalTempFromBias calc: PERFORM, OMIT, COMPLETE

Table 2.4: Science Data File Primary Header Keywords

Keyword Name	Meaning
<i>Bias-Derived Temperature Calibration Indicators</i>	
TFBDONE	CalTempFromBias calc: PERFORM, OMIT, COMPLETE
<i>Calnica Calibration Reference Files (inputs to calnica)</i>	
MASKFILE	Static data quality file
NOISFILE	Detector read noise file
NLINFILE	Detector non-linearity file
DARKFILE	Dark current file
TEMPFILE	Temperature dependent dark file
LINSCALE	Scaling factor for linear image
AMPSCALE	Scaling factor ampglow image
FLATFILE	Flat field file
TDFFILE	Temperature-dependent flat field
TDFGROUP	Imset from TDFFILE applied by calnica
PHOTTAB	Photometric calibration table
BACKTAB	Background model parameters table
IDCTAB	Image distortion correction table
<i>Calnica Calibration Reference File Pedigree (outputs from calnica)</i>	
MASKPDGR	Static data quality file pedigree (values: GROUND dd/mm/yyyy - for reference files originated from Thermal Vacuum data; INFLIGHT dd/mm/yyyy - for reference files originated from on-orbit calibration observations)
NOISPDGR	Detector read noise file pedigree (values: GROUND dd/mm/yyyy; INFLIGHT dd/mm/yyyy)
NLINPDGR	Detector non-linearity file pedigree (values: GROUND dd/mm/yyyy; INFLIGHT dd/mm/yyyy)
DARKPDGR	Dark current file pedigree (values: GROUND dd/mm/yyyy; INFLIGHT dd/mm/yyyy; and MODEL dd/mm/yyyy for the synthetic darks, see Chapter 3)
FLATPDGR	Flat field file pedigree (values: GROUND dd/mm/yyyy; INFLIGHT dd/mm/yyyy)
PHOTPDGR	Photometric calibration table pedigree (values: GROUND dd/mm/yyyy; INFLIGHT dd/mm/yyyy)
BACKPDGR	Background model parameters table pedigree (values: GROUND dd/mm/yyyy; INFLIGHT dd/mm/yyyy)
<i>Calnica Calibration Switches (allowed values: PERFORM, OMIT)</i>	
BIASCORR	Correct wrapped pixel values
ZSIGCORR	MULTIACCUM zero read signal correction
ZOFFCORR	Subtract MULTIACCUM zero read
MASKCORR	Data quality initialization (DQ array)
NOISCALC	Calculate statistical errors (ERR array)
NLINCORR	Correct for detectors non-linearities
DARKCORR	Dark correction
BARSCORR	Bars correction
FLATCORR	Flat-field correction
UNITCORR	Convert to count rate
PHOTCALC	Populate photometry keywords
CRIDCALC	Identify cosmic ray hits (update of DQ arrays in *_ima.fits output of calnica for MULTIACCUM)
BACKCALC	Calculate background estimates
WARNCALC	Generate user warnings

Table 2.4: Science Data File Primary Header Keywords

Keyword Name	Meaning
<i>Calnica Calibration Indicators (output from calnica; values: PERFORMED, SKIPPED, OMITTED)</i>	
BIASDONE	Correct wrapped pixel values
ZSIGDONE	MULTIACCUM zero read signal correction
ZOFFDONE	Subtract MULTIACCUM zero read
MASKDONE	Data quality initialization (DQ array)
NOISDONE	Calculate statistical errors (ERR array)
NLINDONE	Correct for detectors non-linearities
DARKDONE	Dark correction
BARSDONE	Bars correction
FLATDONE	Flat-field correction
UNITDONE	Convert to count rate
PHOTDONE	Populate photometry keywords
CRIDDONE	Identify cosmic ray hits (update of DQ arrays in *_ima.fits output of calnica for MULTIACCUM)
BACKDONE	Calculate background estimates
WARNDONE	Generate user warnings
CALSTAGE	State of the calibration (values: CALNICA, CALNICB, UNCALIBRATED)
CAL_VER	Version number of the CALNICA (CALNICB) code for _cal.fits (_mos.fits) files
PROCTIME	Pipeline processing time (MJD)
OPUS_VER	OPUS software system version number
<i>Post-SAA Dark Keywords (used with post-SAA darks in Cycle 11+)</i>	
SAA_EXIT	Time of last exit from SAA contour level 23
SAA_TIME	Seconds since last exit from SAA contour 23
SAA_DARK	Association name for post-SAA dark exposures
SAACRMAP ¹	SAA cosmic ray map file
<i>Bright Earth Persistence Keywords</i>	
BEPSCALE	Level of persistence calculated
BEPVALLO	Minimum allowed value of the persistence to apply
BEPUSELO	Minimum allowed fraction of pixels used
BEPFRAC	Fraction of pixels used to calculate persistence
<i>Runcalsaa Calibration Reference Files</i>	
SAADFILE	SAA dark reference image file
SAADPDGR	SAA dark reference file pedigree
SAACNTAB	Saaclean reference table (with task params)
SAACPDGR	Pedigree of saaclean reference table
PEDSBTAB	Pedsub reference table
PDSBPDGR	Pedigree of pedsub reference table
PMODFILE	Persistence model file
PMSKFILE	Persistence mask file
<i>RUNCALSAA Calibration Switches</i>	
SAACORR	Correct for SAA signature
BEPCORR	Calculate and apply bright earth persistence

Table 2.4: Science Data File Primary Header Keywords

Keyword Name	Meaning
<i>RUNCALSAA Calibration Indicators</i>	
SAADONE	Correct for SAA signature
BEPDONE	Calculate and apply bright earth persistence
<i>Saa_clean Output keywords</i>	
SAAPERS	SAA Persistence image
SCNPSCL	Scale factor used to construct persistence image
SCNPMDN	Median used in flatfielding persistence image
SCNTHRS	Threshold dividing high and low signal domains
SCNHNPIX	Number of pixels in high signal domain(HSD)
SCNLNPIX	Number of pixels in low signal domain(LSD)
SCNHCHI2	HSD chi squared for parabola fit
SCNHSCL	HSD scale factor for min noise
SCNHEFFN	HSD effective noise at SCNGAIN
SCNHNRED	HSD noise reduction(percent)
SCNLCHI2	LSD chi squared for parabola fit
SCNLSCL	LSD scale factor for min noise
SCNLEFFN	LSD effective noise at SCNGAIN
SCNLNRED	LSD noise reduction(percent)
SCNAPPLD	To which domains was SAA cleaning applied
<i>RNLINCOR Calibration Reference Files</i>	
ZPRATTAB	Nonlincor zeropoint scaling table
RNLCORTB	Nonlincor nonlinearity power law table
<i>Calnicb Calibration Information</i>	
ILLMCORR	Subtraction of background illumination pattern reference image (input values: PERFORM, OMIT)
ILLMDONE	Subtraction of background illumination pattern reference image (output values: PERFORMED, SKIPPED, OMITTED)
ILLMFILE	Background illumination pattern reference image filename
ILLMPDGR	Background illumination pattern file pedigree
MEAN_BKG	Mean background level (DN/sec), computed by calnicb
<i>Pattern Keywords</i>	
PATTERN1	Primary pattern type
P1_SHAPE	Primary pattern shape
P1_PURPS	Primary pattern purpose
P1_NPTS	Number of points in primary pattern
P1_PSPAC	Point spacing for primary pattern (arc-sec)
P1_LSPAC	Line spacing for primary pattern (arc-sec)
P1_ANGLE	Angle between sides of parallelogram pattern (deg)
P1_FRAME	Coordinate frame of primary pattern (POS-TARG or CELESTIAL)
P1_ORIENT	Orientation of pattern to coordinate frame (deg)
P1_CENTER	Center pattern relative to pointing (yes/no)
BKG_OFF	Pattern offset method (SAM or FOM)
PATTSTEP	Position number of this point in the pattern
PATT_POS	Position number in pattern sequence

Table 2.4: Science Data File Primary Header Keywords

Keyword Name	Meaning
Target Acquisition Keywords (useful for Coronagraphic Data)	
NCHKBOXX	CHeckBOX location X
NCHKBOXY	CHeckBOX location Y
NTABOXSZ	TA checkBOX SiZe
NXCENT	X pos CENTroid (steps)
NYCENT	Y pos CENTroid (steps)
NXCENTP	X pos CENTroid (pixels)
NYCENTP	Y pos CENTroid (pixels)
NBOXSUM	checkBOX SUM
NOFFSETX	OFFSET maneuver X (steps)
NOFFSETY	OFFSET maneuver Y (steps)
NOFFSTXP	OFFSET maneuver X (pixels)
NOFFSTYP	OFFSET maneuver Y (pixels)
NSLEWCON	SLEW CONfiguration (Clear, Set)
Association Keywords	
ASN_ID	Association rootname
ASN_TAB	Name of the association table
ASN_MTyp	Role of the dataset in the association (e.g., target, first background, second background, etc.; allowed values: EXP_TARG, EXP_BCKn, PROD_TARG, PROD_BCKn, where EXP=input exposure, PROD=output product, TARG=target, BCK=background, n=1-8)

1. The SAACRMAP keyword is no longer being used by the OTFR pipeline.

In the SCI image extensions, additional keywords describing the data quality are present. They give the number of pixels which have a flag different from zero in the DQ extension, and a suite of statistical information (mean, standard deviation, minimum and maximum of good pixels in the entire detector and per quadrant) on the image. Table 2.5 lists some of the relevant keywords that are specific to image extensions; they appear in the extension headers, but not in the primary header.

Table 2.5: Image Extension Header Keywords in Science Data Files

Keyword Name	Meaning
Data Description Keywords	
EXTNAME	Name of the extension in an imset of the data file (SCI, ERR, DQ, SAMP, TIME)
EXTVER	Extension version; integer number to uniquely identify an IMSET in a science data file. A MULTI-ACCUM file can contain up to 26 IMSETs, i.e. up to EXTVER=26.
INHERIT	Switch to allow the image extension header to inherit the primary header keywords. Allowed values: T=TRUE, F=FALSE.
DATAMIN	Minimum pixel value
DATAMAX	Maximum pixel value
BUNIT	Brightness units; allowed values: COUNTS, COUNTS/S.
PIXVALUE	When ALL pixels in an image extension have the same value (e.g., the SAMP and TIME arrays in the *_ima.fits file from a MULTIACCUM exposure or the ERR, DQ, SAMP and TIME arrays in the *_raw.fits file from a MULTIACCUM, ACCUM or BRIGHTOBJ exposure) the pixel array of that extension is not generated, and the PIXVALUE keyword is instead populated with the common value of the pixels to save space.
World Coordinate System of Image	
CRPIX1	x-coordinate of image's reference pixel
CRPIX2	y-coordinate of image's reference pixel
CRVAL1	RA of reference pixel (degrees)
CRVAL2	DEC of reference pixel (degrees)
CD1_1	Partial derivative of RA with respect to x
CD1_2	Partial derivative of RA with respect to y
CD2_1	Partial derivative of Dec with respect to x
CD2_2	Partial derivative of Dec with respect to y
Readout Parameters	
SAMPNUM	Sample number of the MULTIACCUM sequence
SAMPTIME	Total integration time (sec)
DELTATIM	Integration time of the sample (sec)
ROUTTIME	UT time of array readout (MJD)

Keywords in the support file, *_spt.fits, report information from the ephemeris and engineering data on the status of the telescope and of the instrument during the observations. Information common to all readouts of a MULTIACCUM sequence are stored in the primary header of the support file, while information which may change from readout to readout (e.g., detector temperature) is stored in the headers for each corresponding extension. Table 2.6 describes some of the relevant primary header keywords from the *_spt.fits file, and Table 2.7 gives some useful keywords from the extension headers.

Table 2.6: NICMOS Primary Header Keywords in the Support Files

Keyword Name	Meaning
PA_V3	Position angle of the V3 axis of HST (degrees)
RA_V1	RA of the V1 axis of HST (degrees in J2000)
DEC_V1	DEC of the V1 axis of HST (degrees in J2000)
RA_SUN	RA of the Sun (degrees in J2000)
DEC_SUN	DEC of the Sun (degrees in J2000)
RA_MOON	RA of the Moon (degrees in J2000)
DEC_MOON	DEC of the Moon (degrees in J2000)

Table 2.7: Some Useful NICMOS Extension Header Keywords in the Support Files

Keyword Name	Meaning
NDWTMP11	Camera 1 and 2 Mounting Cup temp (deg K)
NDWTMP13	Camera 3 Mounting Cup temp (deg K)

Table 2.8: NICMOS and NCS Telemetry Mnemonics

Mnemonic	MSID	Sample time	Units	Operational limits ^a	Description
MNCIRSPD	M25L563A	60s	rps	0-1250	NCS Clrc Rot SPeeD
MNCORSPD	M25L565A	15s	rps	0-7360	NCS CComp Rot SPeeD
MNCONTRL	M32J991A	60s	K	?-103.344	NCS CONTRoL point temp
MNPDESTPT	M32J993A	60s	K	77.1	NCS PiD SeT Point Temp
MNCRADAT	M26T780A	60s	C	-70-+70	NCS Cpl RAD A Temp
MNHTREJT	M25T788A	60s	C	-45-+45	NCS HeaT REJect Temp
MNPNCOLT	M25T551A	60s	K	?-197.102	NCS Pri NiC OutLet Temp
MNRNCILT	M25T548A	60s	K	?-103.310	NCS Red NiC InLet Temp
MNRNCOLT	M25T547A	60s	K	?-103.420	NCS Red NiC OutLet Temp
NDWTMP11	N12T656A	30s	K	?-77.43	NIC1 Mounting Cup Temp
NDWTMP13	N12T658A	30s	K	?-76.28	NIC3 Mounting Cup Temp
NDWTMP14	N12T659A	30s	K	?-76.81	Cold Well Temp
NDWTMP21	N12T662A	30s	K	48.15-263.15	NIC2 Cold Mask Temp
NDWTMP22	N12T663A	30s	K	48.15-263.15	NIC3 Colds Mast Temp

a. Operational limits are a range of values over which the sensor will operate normally.

2.3 Working with NICMOS Files

The quickest way to learn how each observation was performed is to use the **iminfo** task in the **STSDAS.toolbox.headers** package to look at the headers of the science data. The output from **iminfo** summarizes on one screen the relevant information about an observation (Table 2.9) and the instrument configuration during the observations (Table 2.10), by reading and reporting the values of various keywords.

Table 2.9: Observation Information in **iminfo** Listing

Field Descriptor	Header Keyword Source
Rootname	ROOTNAME
Instrument	INSTRUME
Target Name	TARGNAME
Program	ROOTNAME (positions 2–4)
Observation set	ROOTNAME (positions 5–6)
Observation	ROOTNAME (positions 7–8)
File Type	FILETYPE
Obs Date	DATE-OBS or FPKTTIME
Proposal ID	PROPOSID
Exposure ID	PEP_EXPO
Right Ascension	CRVAL1
Declination	CRVAL2
Equinox	EQUINOX

Table 2.10: NICMOS-Specific Information in **iminfo** Listing

Field Descriptor	Header Keyword Source
Image type	IMAGETYP
Number of extensions	NEXTEND
Camera number	CAMERA
Aperture	APERTURE
Filter name	FILTER
Observation Mode	OBSMODE
Number of initial/final reads	NREAD (ACCUM)
Number of intermediate samples	NSAMP (MULTIACCUM)
MULTIACCUM sequence	SAMP_SEQ

Field Descriptor	Header Keyword Source
Exposure time (sec)	EXPTIME
Readout speed	READOUT
Association ID	ASN_ID
Number of Iterations	NUMITER
Calibration steps done	Switches whose values are set to "PERFORMED". Switches are: ZSIGDONE, ZOFFDONE, MASKDONE, BIASDONE, NOISDONE, DARKDONE, NLINDONE, BARSDONE, FLATDONE, UNITDONE, PHOTDONE, CRIDDONE, BACKDONE, WARNDONE, TFBDONE, SAADONE, BEP-DONE,

The entire suite of keywords from any header can be listed with the **IRAF** task **imheader**. Given that NICMOS data files contain multiple extensions, the number of the desired extension must always be specified. For example, to list the primary header content of a calibrated image, you type

```
cl> imheader n0g70106t_cal.fits[0] long+ | page
```

where [0] identifies the primary header. To list the header of the *second* science image in a MULTIACCUM sequence (the sixth extension):

```
cl> imheader n0g70106t_cal.fits[6] long+ | page
```

Chapter 2 of the "[HST Data Handbook](#)" describes in detail how to work with FITS file extensions. Here we will recap the essentials. In order to simplify access to NICMOS FITS image extensions, each extension header contains the two keywords EXTNAME (extension name) and EXTVER (extension version number). The EXTNAME keyword identifies the nature of the extension (SCI, ERR, DQ, SAMP, TIME, see Table 2.9). The EXTVER keyword contains an integer value which is used to uniquely identify a particular imset (quintuple of image extensions). For example, the five image extensions (single imset) contained in the science data file for an ACCUM or BRIGHTOBJ observation will all usually be assigned an EXTVER value of 1 because there will only be one set of extensions in the file. In a MULTIACCUM science data file, each set of extensions associated with a given readout will have a unique EXTVER value, running from 1 up to the total number of readouts in that particular file.

To list the header of the *second* science image in a MULTIACCUM sequence, in place of the command line above, one could instead type:

```
cl> imheader n0g70106t_cal.fits[sci,2] long+ | page
```

In general, to access a particular image extension, append the name and version number of the desired extension in square brackets to the end of the file name. The `EXTNAME` value is specified first, then the `EXTVER` value, separated by a comma. Indeed, the use of the keywords `EXTNAME` and `EXTVER` is not limited to the task **imheader**, but can be used in all **IRAF** tasks.



The primary header data unit in a NICMOS FITS file does not contain the `EXTNAME` or `EXTVER` keywords. The absolute extension number 0 (zero) refers to the primary header.

If a calibration keyword needs to be changed, the **IRAF/STSDAS** **chcalpar** task can be used. For instance, to modify the flat-field calibration switch from `PERFORM` to `OMIT` in a given data file, the following command can be given:

```
cl> chcalpar n0g70106t_raw.fits
```

The parameter set (or "pset") list appropriate for the image will appear, and the calibration keyword can be modified. The operation performed with **chcalpar** can be equivalently performed (although in a more cumbersome way) with the general **IRAF** task **hedit**; in this case, the extension [0] of the primary header *must* be explicitly specified:

```
cl> hedit n0g70106t_raw.fits[0] flatcorr OMIT
```



Do not try to edit a keyword in an extension header unless you are certain that the keyword does not reside in the primary header.

Image sections can be specified in the case of NICMOS data with the same syntax as all **IRAF** images. For example, to specify a pixel range from 101 to 200 in the *x* direction and all pixels (denoted by an asterisk) in the *y* direction from the second error image in a file, the complete file name specification would be:

```
n0g70106t_cal.fits[err,2][101:200,*].
```



If you use both extension and image section syntax together, the extension name or number must come first, enclosed in one set of brackets, and the image section specification in a second set of brackets.

2.4 From the Phase II Proposal to Your Data

The connection between the Exposure Logsheet that each observer fills out during the Phase II proposal process and the datasets and associations that the observer receives once the observations are executed can be better understood through some examples.

The first example shows an exposure logsheet entry that will generate only one dataset:

```
Exposure_Number: 1
Target_Name: HDF
Config: NIC2
Opmode: MULTIACCUM
Aperture: NIC2
Sp_Element: F160W
Optional_Parameters: SAMP-SEQ=STEP256, NSAMP=12
NUMBER_of_Iterations: 1
Time_Per_Exposure: DEF
Special_Requirements: POS TARG 0.5, 0.5
```

The science data file in the dataset will contain 13 imsets (corresponding to the MULTIACCUM NSAMP=12 parameter plus the 0'th read), and some of the header keywords will be filled with the relevant information from the target and exposure logsheets of the Phase II (e.g., the keywords TARGNAME, RA_TARG, DEC_TARG,...).

The next example shows an exposure logsheet entry that will generate both multiple datasets and an association:

```
Exposure_Number: 1
Target_Name: HDF
Config: NIC2
Opmode: MULTIACCUM
Aperture: NIC2
Sp_Element: F160W
Optional_Parameters: PATTERN=SPIRAL-DITH-CHOP, NUM-POS=8,
DITH-SIZE=1.5, CHOP-SIZE=25.0, SAMP-SEQ=STEP256, NSAMP=12
Number_of_Iterations: 1
Time_Per_Exposure: DEF
Special_Requirements:
```

In this observation, eight datasets (one for each position of the pattern) and one association will be created. The pipeline products will include the eight reduced datasets, one mosaic of the background-subtracted target, and one mosaic of the background.

An association will be generated also in the case below:

```
Exposure_Number: 1
Target_Name: HDF
Config: NIC2
Opmode: MULTIACCUM
Aperture: NIC2
Sp_Element: F160W
Optional_Parameters: SAMP-SEQ=STEP256, NSAMP=12
NUMBER_of_Iterations: 3
Time_Per_Exposure: DEF
Special_Requirements:
```

The number of iterations is 3, implying that three datasets will be generated from this exposure logsheet, plus an association table containing the three datasets. The collection of multiple iterations into an association is a new feature introduced by the NICMOS and STIS pipelines. In our specific example, the co-added image from the three iterations will be one of the products of the pipeline.

2.5 Paper Products

Paper products typically summarize the set of exposures that constitute a visit in the Phase II proposal. The set of exposures can be either individual datasets or associations. Paper products are produced by accessing the appropriate keywords in the dataset headers or in the association tables.

After the data from an observation have been received and processed through the STScI pipeline, PDF files (*paper products*) can be generated which summarize the data obtained. The paper products are generated using the `stsdas.hst_calib.paperprod` task `pp_dads`. Here we briefly describe the NICMOS paper products.

A given page of the NICMOS paper products falls into one of two categories: visit-level page or exposure-level page. The content of the pages is as follows:

Visit-Level Pages

- **Cover Page:** contains the proposal ID, the visit number, the PI's last name, and the proposal title.
- **Explanatory Notes:** a set of notes explaining the information contained in the paper products.
- **Target List:** a table listing the targets of the observations being summarized.
- **Observation Summary:** a table summarizing the proposal information for each exposure in the present set, including processing and data quality flags.
- **Optional Parameters:** a table listing the optional parameters, other than the pattern related parameters, used in the observations.
- **Observing Pattern Strategy:** a table listing the observing pattern used for each exposure in the set.

Exposure-level Pages

- **Final Calibrated Image:** a grey-scale plot of the calibrated science image (a mosaic if the observation was dithered).
- **Observation Parameters:** several useful parameters are listed on the right hand side of a subset of the paper product pages. Observation root name, the date and time of the observation, the target name and position, the instrument configuration, FOM offset, and pattern, dither and chop information is given.

- ***Spacecraft Performance:*** known problems with guide star acquisition, spacecraft guidance, recenterings, and telemetry drop-outs are listed, as are detected problems with the instrument's operation (e.g., Take Data flag NOT on throughout observation).
- ***Pipeline Processing Summary:*** any problems encountered in the routine pipeline processing of the data are listed.
- ***Calibration Data Quality Summary:*** possible problems with the calibration reference files is summarized; for example, any dummy reference files used in the calibration would be identified.
- ***Thumbnail plots:*** the individual exposures for dithered, chopped, and NUMITER > 1 observations are given.
- ***Observing Pattern:*** a schematic (cartoon) of the observing pattern is shown.
- ***Dither, Chip Mosaics:*** plots of the mosaiced calibrated image (on-target) and average mosaiced background image (off-target) are included.
- ***Data Quality Summary:*** a summary of the spacecraft performance, pipeline processing status, and calibration data quality for each exposure.
- ***Calibration Reference File Summary:*** a summary of the calibration processing switches and reference files used to process each exposure.

CHAPTER 3:

Calibration

In this chapter. . .

3.1 Pipeline Processing, OTFR, and the HST Archive / 35

3.2 NICMOS Calibration Software / 37

3.3 Basic Data Reduction / 39

3.4 Mosaicing/Drizzling / 56

3.5 Recalibration / 62

3.6 Calibration Goals and Plans / 67

3.1 Pipeline Processing, OTFR, and the HST Archive

NICMOS data are retrieved from the *HST* Archive using “On-The-Fly Reprocessing” (OTFR), a method also implemented for ACS, STIS and WFPC2, and planned for future instruments (e.g. COS and WFC3). OTFR goes back to the original telemetry (the “POD files”) to reconstruct FITS files, and then processes these raw FITS data through the most up-to-date version of the OPUS pipeline software, using the latest and best reference files available at the time of retrieval from the Archive, regardless of when the observations were conducted. As with all *HST* instruments, the pipeline software and reference files have evolved and improved with time as our knowledge of the instrument and its calibration have developed. OTFR ensures that users will receive the best standard processing available at the time they request NICMOS data from the Archive, and makes it easy to recalibrate data taken earlier in the mission lifetime.


All of the steps performed by the pipeline are recorded in the trailer file for your dataset (`*_trl.fits`). The main steps performed by the pipeline are:

1. The data are partitioned (separated into individual files, e.g., engineering and science data are separated).

2. The data are edited, if necessary, to insert fill values in place of missing data.
3. The data are evaluated to determine if there are discrepancies between a subset of the planned and executed observational parameters.
4. A list of calibration reference files to be used in the calibration of the data is created based on the executed observational parameters. This step does not generate comments in the NICMOS trailer file.
5. The raw data are converted to a generic (FITS) format and the header keyword values are populated (known as *generic conversion*).
6. The raw data is used to calculate the detector temperature at the time of the observation using the CalTempFromBias software.
7. The raw data are calibrated using a standard set of NICMOS calibration programs (**calnica** and **calnicb**).
8. If applicable, the task **runcalsaa** is run

The OTFR processing steps that involve **STSDAS** routines are described in Figure 3.1.

Figure 3.1: Processing Flow for OTFR

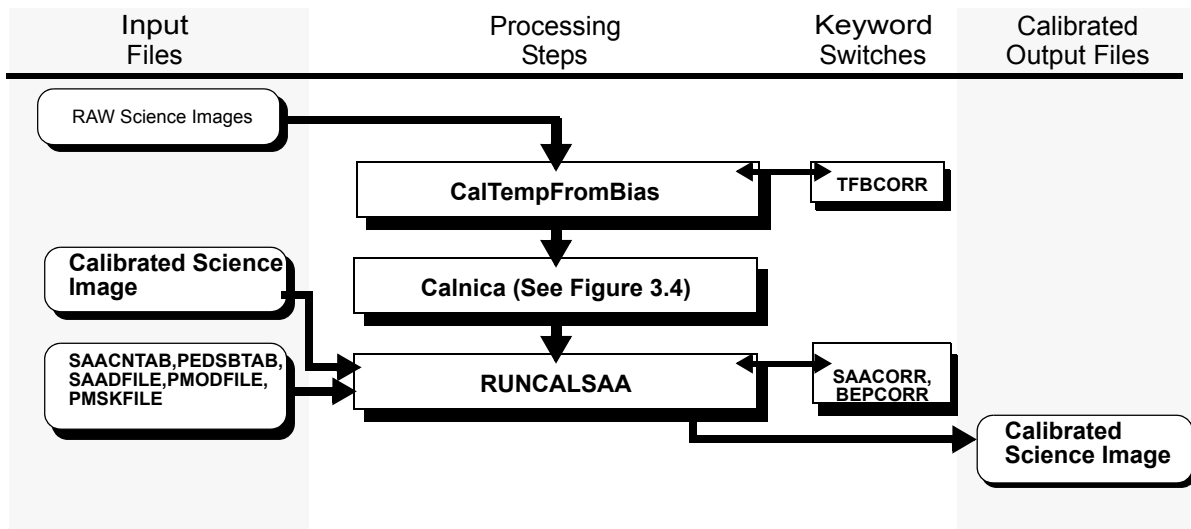

The calibration software used by the pipeline (steps 6-8 above) is exactly the same as that provided within **STSDAS** (see Section 3.2). The calibration files and tables used are taken from the Calibration Data Base System (CDBS) at STScI and are the most up-to-date versions available at the time the data are requested and processed by OTFR. However, calibration reference files and software have been improved with time,

which is a reason why you may wish to reprocess your data. For example, beginning 17 December 2008 (OPUS version 2008_a and later), the data retrieved using OTFR uses temperature dependent reference files in the calibration step. Also, prior to 26 September 2001, the HST archive did not use the OTFR, so if you received NICMOS data as a GO or from the HST Archive before that date, the reference files and software used may be outdated. Therefore if you require best possible calibrations, you should check the retrieval status of your data and possibly consider recalibration. This is further described in Section 3.5

3.2 NICMOS Calibration Software

3.2.1 The Calibration Pipeline

The science data that an observer receives are calibrated in the pipeline by the following **STSDAS** calibration routines: **CalTempFromBias**, **calnica**, **calnicb** and **runcalsaa**. These routines perform different operations:

1. **CalTempFromBias**: This routine calculates the temperature of the detector from the measured bias levels. It runs only on the MULTI-ACCUM observations and runs on the *_raw.fits files.
2. **calnica**: This routine removes the instrumental signature from the science data. It is the first calibration step, and is applied to *all* NICMOS datasets individually. **Calnica** operates on the raw science data files.
3. **calnicb**: This routine operates on *associations*: it co-adds datasets obtained from multiple iterations of the same exposure, mosaics images obtained from dither patterns, and background-subtracts images obtained from chop patterns. **Calnicb** is applied to the calibrated science data files (output from **calnica**), and requires association tables (*_asn.fits) and the telemetry and engineering data files (*_spt.fits)
4. **Runcalsaa**: This routine measures and removes an estimate of the SAA persistence signal and Bright Earth Persistence signal in a NICMOS image

These routines determine which calibration steps are to be performed by looking at the values of the *calibration switch* keywords in the primary header of the input science data files (see Table 2.4). The tasks select the reference files to use in the calibration of the data by retrieving the reference file names from the *reference file* keywords, also located in the

primary header of the input data files. The appropriate values of the calibration switches and reference file keywords depend on the instrumental configuration used, the date when the observations were taken, and any special pre-specified constraints. They are set in the headers of the raw data file in the pipeline during the generic conversion process. The *calibration indicators* keywords record which steps have been performed on the data, and get updated after processing. In particular, the indicators for completed steps will have been assigned the value “PERFORMED”, while the indicators for the steps that were not performed will have been set to “OMITTED” or “SKIPPED”. If the calibration switch keyword is set to “OMIT,” then the calibration indicator keyword will be “OMITTED” after running the calibration routine. If the calibration switch keyword is set to “PERFORM,” and the reference file is a dummy, then the calibration indicator keyword will be “SKIPPED.” The calibration indicators keywords should be examined in the primary header of the calibrated science data (*_cal.fits) to determine what calibration steps were applied to the data.

The **CalTempFromBias**, **calnica**, and **calnicb** tasks are available in **STSDAS** in the **hst_calib.nicmos** package. The **runcalsaa** routine in the pipeline comprises of two **PyRAF** tasks, **saaclean** and **nic_rem_persist** which are also available in the **hst_calib.nicmos** package. By using these tasks, observers can recalibrate data using the same software as the routine calibration pipeline at STScI. As an alternative, users who want to combine dithered or mosaiced NICMOS images can use the **MultiDrizzle** software:

(<http://stsdas.stsci.edu/multidrizzle/>)

3.2.2 Software for Grism Data Reduction

The NICMOS grism mode permits multi-object, slitless spectroscopy at low resolution. The **calnica** pipeline will process such grism images but will not apply the flat-fielding step. NICMOS flat fields strongly depend on wavelength, flat-fielding of grism data therefore needs to take the wavelength of extracted spectra into account. Software to extract spectra from **calnica** processed images is available from the Space Telescope European Coordinating Facility (ST-ECF).

Two software packages are available:

1. **NICMOSlook**. This is an interactive GUI driven **IDL** program to extract spectra from pairs of NICMOS grism images and corresponding undispersed images. It has a range of options to address specific properties of the NICMOS detector. It is the recommended program to extract individual spectra from NICMOS grism data. Program and documentation are available for reference at:

<http://www.stecf.org/instruments/NICMOSgrism/nicmoslook/nicmoslook>

2. **aXe**. This is a non-interactive general purpose package to extract spectra from slitless spectroscopy data. It can either be run stand-alone or within **PyRAF**. A version of **aXe** which includes correction for NICMOS specific effects and NICMOS configuration files is available. **aXe** is the program of choice to extract a large number of spectra from several images simultaneously. It is available at:

<http://www.stecf.org/instruments/ACSgrism/axe/>

Both packages require special NICMOS grism calibration data which are distributed with software. The packages are supported by the ST-ECF and questions should be directed to stdesk@eso.org

Because NICMOS grism data processing and extraction are not really "pipeline" procedures, this handbook will defer an overview of grism reduction methodology and the software tools **calnirc** and **NICMOSlook** until Chapter 5, where the discussion of NICMOS Data Analysis is presented.



You cannot run NICMOSlook unless you have an IDL licence.

3.3 Basic Data Reduction

3.3.1 CalTempFromBias


Before the *_raw.fits images are processed by **calnica**, the temperature as determined from the detector bias levels is calculated using the **STSDAS** task **CalTempFromBias** for all images taken with MULTIACCUM mode (the only mode for which the method works). This step is attempted by default (TFBCALC = 'PERFORM') and results in a keyword setting TFBDONE = 'PERFORMED' if the task succeeds. The resulting temperature is assigned to the TFBTEMP keyword. TFBCALC makes it possible to accurately select temperature dependent calibration products when calibrating (e.g. dark correction, flat-field correction and photometric calibration) NICMOS MULTIACCUM mode data.

CalTempFromBias uses the fact that the NICMOS bias levels are temperature dependent. The detector can be thought of as a simple diode in this case and the first read of a MULTIACCUM NICMOS exposure (before light reaches the detector) can be used to compute a temperature of the actual detector at the time the exposure was started. This method is believed to result in more accurate temperatures (accurate to within 0.05K) than those reported by the mounting cup sensors. It also produces more

precise temperature estimates since the temperatures reported by the mounting cup sensor have been observed to slowly diverge from the real temperatures during the last few years. The bias-derived temperature shows that there has been a drift in the detector temperature during the years 2002 to 2008 (for all detectors). This is shown for NIC 1 in Figure 3.2, where the bias-derived temperature (TFBTEMP) is plotted together with the mounting cup temperature (NDWTMP11) as a function of date for a number of dark images. The drift in temperature is about $\Delta t \sim 2\text{K}$ for TFBTEMP. Note that the normalization of TFBTEMP is arbitrary using this method, but the relative evolution of TFBTEMP with time gives a measurement of temperature changes. For further updates please refer to the NICMOS Web page at:

<http://www.stsci.edu/hst/nicmos>

Figure 3.2: Temperature for Individual Dark Images

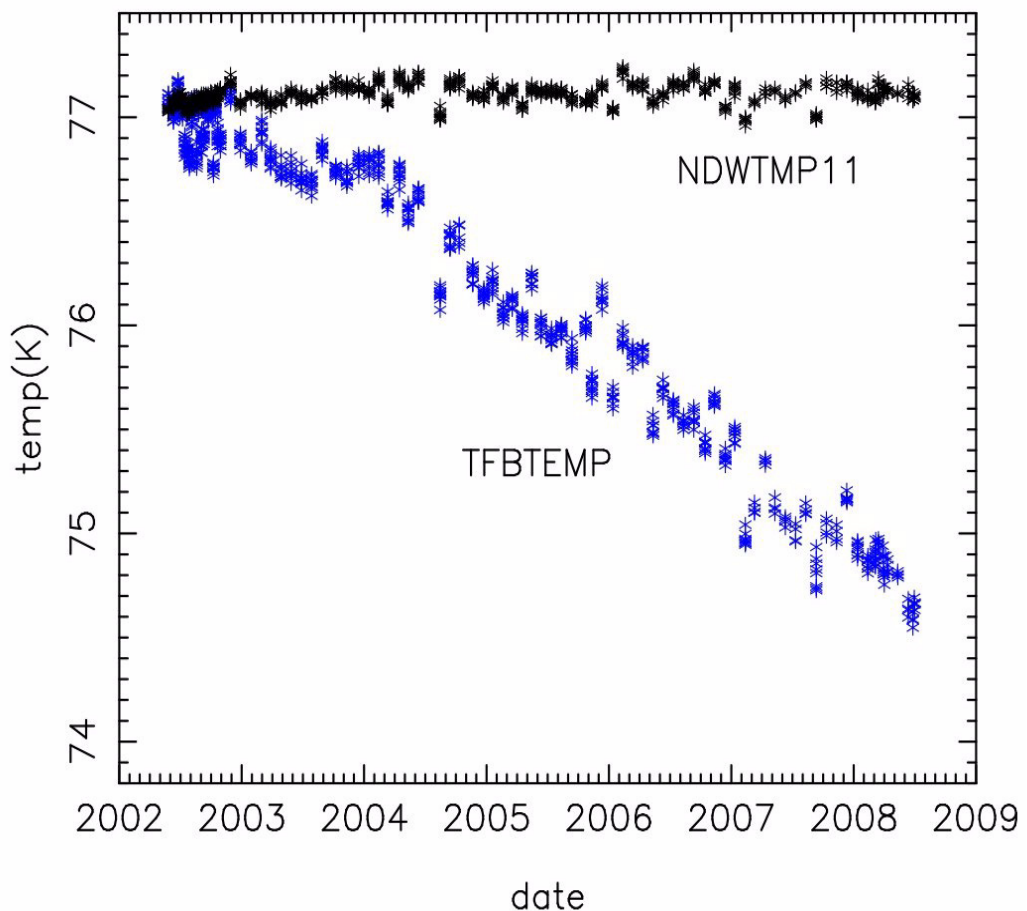

3.3.2 CALNICA

The **calnica** task operates on individual NICMOS datasets and performs the job of removing the instrumental signature from the raw science data. The **calnica** task also tries to identify cosmic ray hits and combines the multiple readouts in MULTIACCUM observations.

The inputs to **calnica** are the raw science (**_raw.fits*) files. The output of **calnica** is usually a single file containing the *calibrated* science data (**_cal.fits*). For MULTIACCUM mode datasets there is an additional intermediate output file (**_ima.fits*) which contains the *calibrated* data from all the intermediate readouts. The *_ima.fits* data are fully calibrated up to, but not including, the cosmic ray rejection. The format of the input and output science data files are identical, so that the output data can be reused as input to **calnica**, if desired. One could, for example, process a science data file through some subset of the normal calibration steps performed by **calnica**, examine or modify the results, and then process the data through **calnica** again, performing other calibration steps or using alternate calibration reference files. One example of such a procedure would be reducing data where there are significant changes in the quadrant bias level from readout to readout in a MULTIACCUM sequence. In Section 4.2, we discuss this common NICMOS data anomaly, and in Section 4.2.4 we describe one technique for treating it using the **biaseq** task. At present, the use of this routine requires multiple, re-entrant applications of **calnica** in order to partially process the images before and after the use of the **biaseq** task.

Figure 3.3 shows the portion of a calibrated NICMOS science file header containing the switches and reference file keywords that pertain to the processing performed by the OTFR. The accompanying flow chart (Figure 3.4) shows the sequence of **calnica** calibration steps, the input data and reference files and tables, and the output data file. Each calibration step is described in detail in the following sections.

Figure 3.3: Partial NICMOS Header

```

/ CALNICA CALIBRATION REFERENCE FILES
MASKFILE= 'nref$m9c1047sn_msk.fits' / static data quality file
NOISFILE= 'nref$mc91052en_noi.fits' / detector read noise file
NLINFILE= 'nref$sav0411gn_lin.fits' / detector nonlinearities file
DARKFILE= 'nref$shbp2024bn_drk.fits' / dark current file
TEMPFILE= 'nref$sc31741nn_tdd.fits' / temperature-dependent dark file
LINSSCALE= 1.000000E+00 / scaling factor for linear image
AMPSCALE= 9.9658579E-01 / scaling factor for ampglow image
FLATFILE= 'nref$sbj1739jn_flat.fits' / flat field file
TDFFILE= 'nref$sbj19224n_tdf.fits' / temperature-dependent flat field
TDFGROUP= 2 / imset from TDFFILE applied by CALNICA
PHOTTAB= 'nref$sbil622en_pht.fits' / photometric calibration table
BACKTAB= 'N/A' / background model parameters table

IDCTAB= 'nref$sd1954tn_idc.fits' / Image Distortion Correction table

/ CALNICA CALIBRATION REFERENCE FILE PEDIGREE
MASKPDGR= 'INFLIGHT 01/07/2002' / static data quality file
NOISPDGR= 'INFLIGHT 01/05/2002' / detector read noise file
NLINPDGR= 'INFLIGHT 02/05/2002' / detector nonlinearities f
DARKPDGR= 'INFLIGHT 14/10/2002 13/08/2008' / dark current file pedigree
FLATPDGR= 'INFLIGHT 30/04/2002 25/07/2008' / flat field file pedigree
PHOTPDGR= 'INFLIGHT 01/01/2002' / photometric calibration t
BACKPDGR= ' ' / background model paramete


/ CALNICA CALIBRATION SWITCHES: perform,omit
BIASCORR= 'PERFORM' / subtract ADC bias level
ZSIGCORR= 'PERFORM' / Zero read signal correction
ZOFFCORR= 'PERFORM' / subtract MULTIACCUM zero read
MASKCORR= 'PERFORM' / data quality initialization
NOISCALC= 'PERFORM' / calculate statistic errors
NLINCORR= 'PERFORM' / correct for detector nonlinearities
DARKCORR= 'PERFORM' / dark correction
BARSCORR= 'PERFORM' / bars correction
FLATCORR= 'PERFORM' / flat field correction
UNITCORR= 'PERFORM' / convert to count rates
PHOTCALC= 'PERFORM' / calculate photometric keywords
CRIDCALC= 'PERFORM' / identify cosmic ray hits
BACKCALC= 'PERFORM' / calculate background estimates
WARNCALC= 'PERFORM' / generate user warnings

/ CALNICA CALIBRATION INDICATORS: performed, skipped, omitted
BIASDONE= 'PERFORMED' / subtract ADC bias level
ZSIGDONE= 'PERFORMED' / Zero read signal correction
ZOFFDONE= 'PERFORMED' / subtract MULTI-ACCUM zero read
MASKDONE= 'PERFORMED' / data quality initialization
NOISDONE= 'PERFORMED' / calculate statistic errors
NLINDONE= 'PERFORMED' / correct for detector nonlinearities
DARKDONE= 'PERFORMED' / dark correction
BARSDONE= 'PERFORMED' / bars correction
FLATDONE= 'PERFORMED' / flat field correction
UNITDONE= 'PERFORMED' / convert to count rates
PHOTDONE= 'PERFORMED' / calculate photometric keywords
CRIDDONE= 'PERFORMED' / identify cosmic ray hits
BACKDONE= ' ' / calculate background estimates
WARDONE= ' ' / generate user warnings

CALSTAGE= 'CALNICA' / state of calibration
CAL_VER= 'Version 4.4.0' / CALNIC code version
PROCTIME= 5.488880490741E+04 / Pipeline processing time (MJD)
OPUS_VER= 'OPUS 2009_1' / OPUS software system version number

```

Figure 3.4: Calnica Processing Flow for a MULTIACCUM Observation

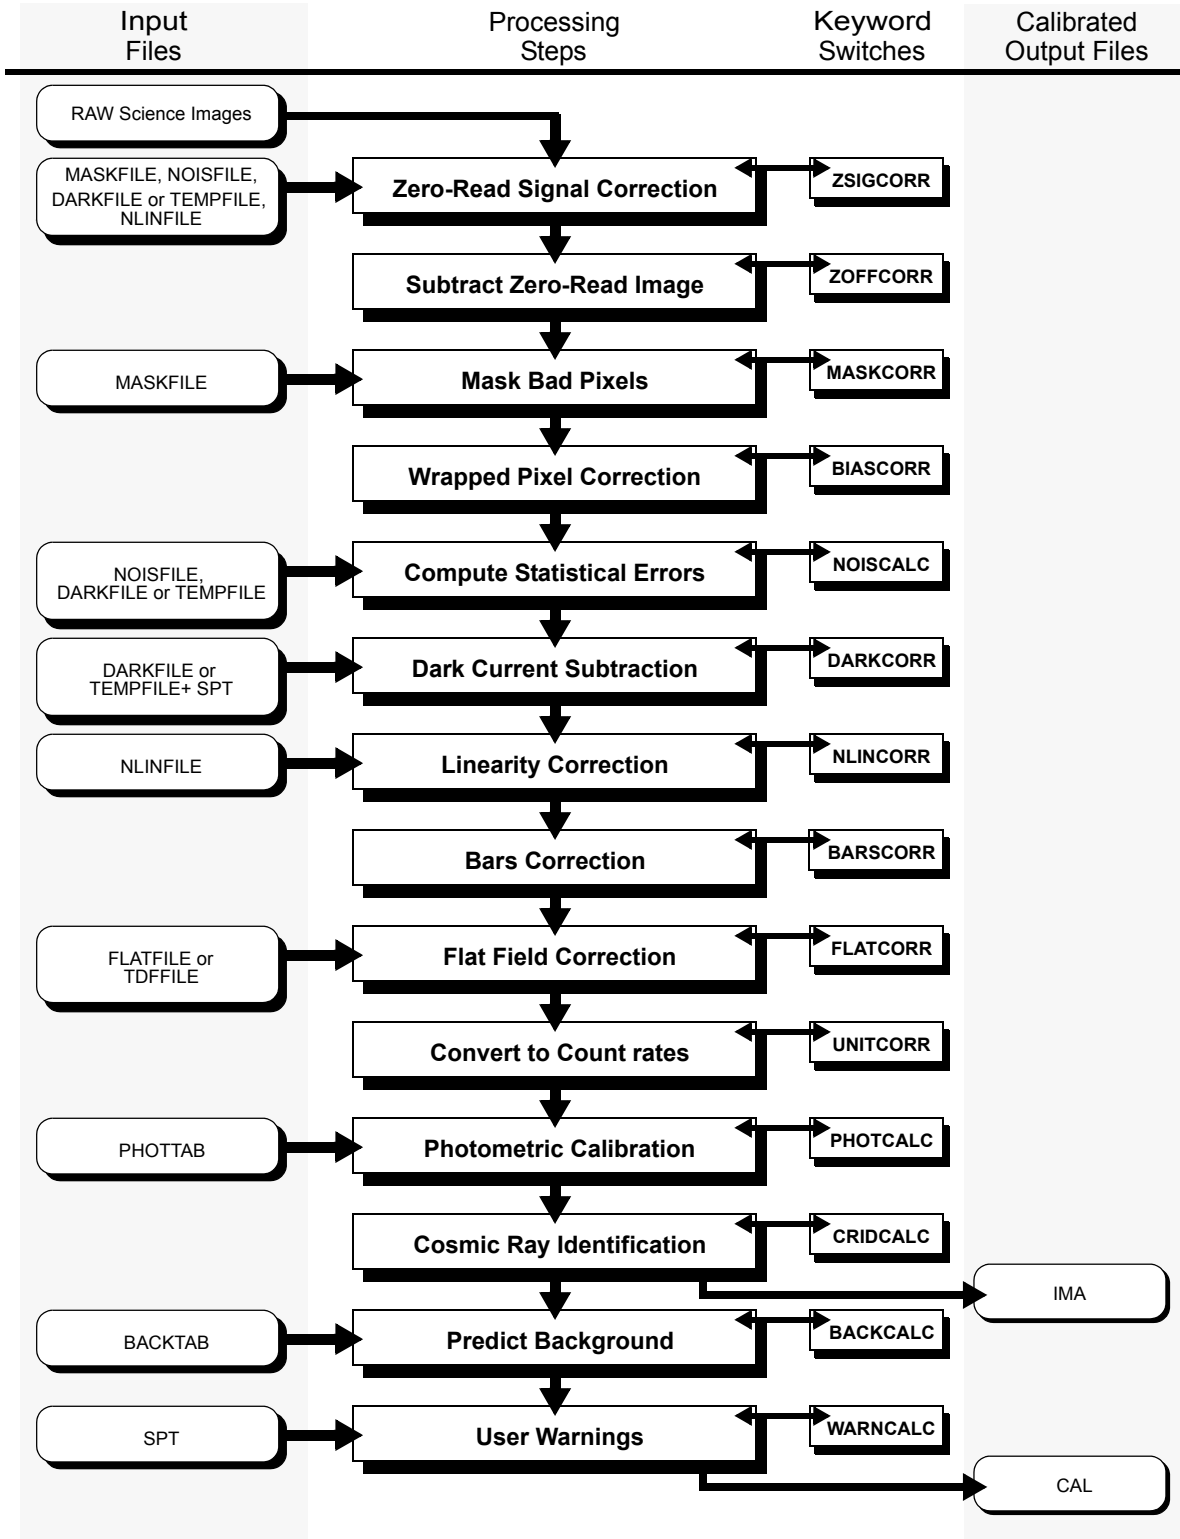

ZSIGCORR (Zero-Read Signal Correction)

At the beginning of a NICMOS observation the detector pixels are reset to a bias level and then read out to record that bias level. There is an interval of approximately 0.2 seconds that elapses between the time each pixel is reset and then read. Because NICMOS does not have a shutter, signal from external sources starts to accumulate during that 0.2 second interval. When the initial (or “zeroth”) read is later subtracted from subsequent readouts, any signal in the zeroth read will also be subtracted. For very bright sources, the amount of signal in the zeroth read can be large enough to lead to inaccurate linearity corrections, as well as the failure to detect saturation conditions in the NLINCORR calibration step, because the linearity correction and saturation checking both depend on the absolute signal level accumulated in a pixel.

For MULTIACCUM observations, the ZSIGCORR step is used to estimate the amount of source signal in the zeroth read and to supply this estimate to the NLINCORR step for linearity corrections. The ZSIGCORR step estimates the amount of signal in the zeroth read by first measuring the amount of signal that arrived in each pixel between the zeroth and first reads, and then scaling that signal to the effective exposure time of the zeroth read (nominally 0.203 seconds). Pixels that have an estimated zeroth read signal greater than 5 times their ERR value are assumed to contain detectable signal; those below this threshold are ignored. (The ERR value for each pixel is the error in the fit through the MULTIACCUM sequence.) The user may set a different zero-read detection threshold by using the `zsthresh` task parameter for **calnica**. The estimated zeroth read signal is then passed, on a pixel-by-pixel basis, to the NLINCORR step, so that it can account for that signal when applying linearity corrections and saturation checking on the zeroth-read subtracted images with which it works. The ZSIGCORR step also performs saturation checking on the zeroth and first readout images.

Note that this technique will not work well for pixels covered by targets that are so bright that the signal is already beginning to saturate in either the zeroth or first readouts.

Pixels that are determined to have detectable signal in the zeroth read are marked in the DQ images of the output `*_cal.fits` and `*_ima.fits` file with a data quality flag value of 2048. The ZSIGCORR routine uses the MASKFILE, NOISFILE, DARKFILE or TEMPFILE, and NLINFILE reference files.



The ZSIGCORR routine is implemented in calnica versions 3.0 and higher. It was implemented in the standard OPUS calibration pipeline on 11 November 1997, and archived data from before that time does not have the ZSIGCORR step applied. If you are concerned about accurate flux measurements for bright sources in NICMOS observations taken before that time, you may wish to reprocess the data using the latest version of calnica (see Section 3.5), or to retrieve the data again from the HST Archive via OTFR, which will automatically apply the ZSIGCORR step.

ZOFFCORR (Subtract Zero-Read Image)

The ZOFFCORR step of **calnica** performs the subtraction of the zeroth read from all readouts in a MULTIACCUM file. This step is performed for data generated by the MULTIACCUM readout mode only. For ACCUM and BRIGHTOBJ readout modes, the subtraction of the zeroth read is performed on-board, because the images returned to the ground are formed by taking the difference of initial and final non-destructive detector readouts.

The pipeline will subtract the zeroth read image from all readouts, including the zeroth read itself. Furthermore, the self-subtracted zeroth-read image will be propagated through the remaining processing steps and included in the output products, so that a complete history of error estimates and data quality (DQ) flags is preserved. After this step is performed, the science data are in the same form as the raw science data from any other observing mode and are processed the same way throughout the remaining steps of **calnica**. No reference files are used by this step.

MASKCORR (Mask Bad Pixels)

Flag values from the static bad pixel mask file are added to the DQ image. This uses the MASKFILE reference file, which contains a flag array for known bad (hot or cold) pixels with flag value DQ = 32. There is one MASKFILE for each detector. Besides the truly “defective” bad pixels included in the MASKFILE reference images there are other bad pixels, for example, pixels affected by “grot” (see Section 4.7.1). In the MASKFILE, pixels affected by “grot” have a flag value DQ = 16.

BIASCORR (Wrapped Pixel Correction)

NICMOS uses 16-bit analog-to-digital converters (ADCs), which convert the analog signal generated by the detectors into signed 16-bit integers. Because the numbers are signed and because the full dynamic range of the converter output is used, raw pixel values obtained from

individual detector readouts can range from -32768 to $+32767$ DN. In practice the detector bias level is set so that a zero signal results in a raw value on the order of -23000 DN. In ACCUM and BRIGHTOBJ modes, where the difference of initial and final readouts is computed on-board, the subtraction is also performed in 16-bit arithmetic. Therefore, it is possible that the difference between the final and initial pixel values for a bright source could exceed the dynamic range of the calculation, in which case the final pixel value will wrap around the maximum allowed by the 16-bit arithmetic, resulting in a negative DN value.

The BIASCORR step searches for pixel values in the range -23500 to -32768 DN and adds an offset of 65536 DN to these pixel values to reset them to their original real values. The BIASCORR step only affects ACCUM and BRIGHTOBJ mode observations, although it is applied to all NICMOS data sets. For MULTIACCUM data, it should have no effect.

No reference files are used by this step.

NOISCALC (Compute Statistical Errors)

The errors of the calibrated NICMOS images are stored in the ERR extension. The way errors are calculated depends on the observing mode and resulting file type (*_cal.fits or *_ima.fits files).

Errors for *_ima.fits files from the MULTIACCUM mode and the ACCUM and the BRIGHTOBJECT modes are calculated using the NOISCALC step. This performs the task of computing an estimate of the errors associated with the raw science data based on a noise model for each detector. Currently the noise model is a simple combination of detector read noise and Poisson noise in the signal, such that:

$$\sigma = \frac{\sqrt{\sigma_{rd}^2 + \text{counts} \cdot \text{adcgain}}}{\text{adcgain}} \text{ (DN)}$$

where σ_{rd} is the read noise in units of electrons, *adcgain* is the analog-to-digital conversion gain factor in electrons per DN (given by header keyword ADCGAIN). Noise is computed in units of electrons, but the result is converted to units of DNs for storage in the error image. The detector read noise is read pixel-by-pixel from the NOISFILE reference image. The data quality flags set in the DQ image of the NOISFILE are propagated into the DQ images of all image sets (imsets) being processed.

Because the noise calculation is performed before dark subtraction has taken place, the noiseless electronic signal component known as “shading” (see DARKCORR below) is still present in the data. In **calnica** versions 3.3 and later the NOISCALC step estimates the level of the shading signal in the data by computing column or row statistics in the DARKFILE reference file. The computed shading estimate is subtracted from the signal in the science image when computing Poisson noise on the detected counts. This yields a more accurate noise estimate than what was produced in earlier versions of the pipeline.

For the calibrated MULTIACCUM *_cal.fits files, the errors represent the uncertainties in the linear fit of the count vs. time in the up-the-ramp sampling for each individual pixel. This is calculated in the CRIDCALC step of **calnica**. Prior to **calnica** version 4.2, Poisson statistics were used in the linear fit of the up-the-ramp scaling. However, this in combination with a non-optimal weighting applied, led to errors that do not truly represent the total errors.

For images using **calnica** version 4.2 and later, a new optimal weighting scheme is applied which does not include Poisson statistics. This gives errors that represent the effective read-noise, but do not include the Poisson errors. More about the rationale for this update is described in NICMOS [ISR 2008-002](#). While the errors only include the read-noise, it is possible for a user to add the Poisson contribution by hand after running **calnica**. To do this, add in quadrature the Poisson contribution to the errors already in the ERR extension. In the default case, where the count rate in the SCI extension is normalized to counts/s, the Poisson contribution will be:

$$\sqrt{(SCI)/(acdgain \times TIME)}$$

where the exposure time is given by the TIME extension and acdgain is the gain factor. Since the errors in the ERR extension represent the read noise, the total error including both Poisson and read noise contributions can be calculated as

$$ERR(total) = \sqrt{\frac{SCI}{acdgain \times time} + ERR^2}$$

Throughout the remaining steps in **calnica**, the error image is processed in lock-step with the science image, getting updated as appropriate. Errors are mostly propagated through combination in quadrature.

In general, the values in the error images should only be regarded as an estimate of the data uncertainties. The precise pixel noise values in NICMOS images are difficult to compute a priori because many factors may contribute, sometimes in unpredictable ways (see, e.g. the discussions of data anomalies such as cosmic ray persistence in Chapter 4).



In general, the values in the error images should only be regarded as an estimate of the data uncertainties. The precise pixel noise values in NICMOS images are difficult to compute a priori because many factors may contribute, sometimes in unpredictable ways (see, e.g., the discussions of data anomalies such as cosmic ray persistence in Chapter 4).

DARKCORR (Dark Current and Bias Shading Subtraction)

Dark images taken with NICMOS contain three distinct, additive signal components: the so-called “shading”, the amplifier glow, and the true dark current. The shading is a noiseless signal that appears as gradient across a detector quadrant and is due to the fact that the bias level on the pixels is gradually changing as they are being read out. The amplitude of the shading signal is a function of the time since a pixel was last read out. The amplifier glow is a signal produced by a small amount of infrared radiation from the detector readout amplifiers. The amplitude of the amplifier glow is directly proportional to the total number of readouts in an observation. The true detector dark current signal is quite small for the NICMOS arrays and is linearly dependent on the total exposure time of an observation. All three signal components are also more or less dependent on detector temperature.

Because the shading and amplifier glow signals depend on factors other than the exposure time of an observation, it is *not* possible to apply a simple scaling of a single dark reference image to match the exposure time of the science data that is being calibrated. To solve this **calnica** originally used a library of dark current images for each of the three cameras, covering all of the predefined MULTIACCUM sample sequences, and a subset of ACCUM exposure times and NREAD values. The reference dark file appropriate for the exposure sequence used in MULTIACCUM, or the exposure time and NREAD values used in ACCUM, is determined by the OPUS generic conversion process when it populates the DARKFILE reference file keyword in the primary header of raw data files. The **calnica** DARKCORR step subtracts the dark reference images, readout-by-readout for MULTIACCUM observations, from the science data. Error estimates of the dark current, stored in the ERR images of the DARKFILE, are propagated in quadrature into the ERR images of all processed science imsets. Data quality (DQ) flags set in the DARKFILE are also propagated into the DQ images of all processed imsets.

One disadvantage with these DARKFILE reference files is that they do not include any temperature dependence of the dark signal. To also include this, new temperature dependent TEMPFILE reference files have been created. There is one such dark reference file for each camera and each file includes the linear dark, the amp glow and the shading components in different extensions. This makes it possible to scale the different components individually in the DARKCORR step in **calnica**, including a scaling for the temperature dependence.

Images taken in Cycles 7 and 7N that are retrieved after March 2002 have the TEMPFILE keyword set. This is also the case for images in Cycle 11 and later if retrieved after September 2002. However, for the latter images, the full temperature dependence of all components was not implemented until May 2009. If both the DARKFILE and TEMPFILE keywords are set in the header of the *_raw.fits file, then **calnica** uses the TEMPFILE in the

DARKCORR step. For images retrieved before the dates given above, where only the DARKFILE exists, observers may want to consider using the OTFR to download their images again to include the temperature dependence of the dark signal in the image calibration.

For BRIGHTOBJ mode data, dark subtraction is skipped by default in **calnica**, because in general the short exposure times should result in insignificant dark current relative to the object signal. In practice there may be bias components with non-zero amplitude (e.g., akin to "shading") which are present in BRIGHTOBJ mode data. At present, however, there is no standard procedure for removing these. Given the very limited use of BRIGHTOBJ mode for on-orbit science, we will not discuss its reduction further here.



Chapter 4 includes a more detailed discussion of NICMOS dark and bias components, their properties and behavior, including irregularities which are not well handled by the standard processing pipeline, and which require special care on the part of the user. Proper removal of additive instrumental signatures (i.e. dark and bias) can be one of the most important steps in achieving high quality, science grade NICMOS data reductions, and we recommend that the user read the relevant sections of Chapter 4 in detail.

NLINCORR (Linearity Correction)

The linearization correction step corrects the integrated counts in the science image for the non-linear response of the detectors. The observed response of the detectors can conveniently be represented by 2 regimes:

- At low and intermediate signal levels the detector response deviates from the incident flux in a way that is correctable using the following expression:

$$F_c = (c_1 + c_2 \times F + c_3 \times F^2) \times F$$

- where c_1 , c_2 and c_3 are the correction coefficients, F is the uncorrected flux (in DN) and F_c is the corrected flux. In practice the coefficient c_1 is set to 1, so that the total correction factor starts at a value of 1 at the zero signal level.
- At high signal levels—as saturation sets in—the response becomes highly non-linear and is not correctable to a scientifically useful degree; the saturation levels are about 21,500 DN (NIC1), 22,500 DN (NIC2), and 26,200 DN (NIC3).

The NLINCORR step applies the linearity correction to pixels with signal below their defined saturation levels. However, it applies no correction to pixels in the high signal regime, but rather flags them in the DQ image as saturated (DQ value = 64). This step uses the NLINFILE reference file, which consists of a set of images containing the c_1 , c_2 , and c_3 correction coefficients and their variances at each pixel. The [NODE, 2] extension of the NLINFILE sets the saturation value for each pixel. Error estimates on the correction applied to non-saturated pixels are propagated into the ERR images of all imsets processed. Data quality flags set in the NLINFILE are also propagated into the processed DQ images. There is one NLINFILE per detector. See also Section 4.4 and Section 4.5 for further discussion on non-linearity issues, including also count-rate non-linearity.

Early versions of NICMOS non-linearity correction used a linear correction scheme. Starting in calnica v3.3 (September 26, 2001), the NLINCORR step was updated to accommodate the 2nd-order correction¹, but is backwards-compatible such that old NLINFILES using the linear correction may still be used if desired. Additionally, the non-linearity reference files include a [NODE,1] extension which sets the data value below which no nonlinearity correction is applied. Currently, the [NODE,1] values are uniformly set to 0.0, reflecting NICMOS nonlinearity at all count levels. However, NLINFILES retrieved prior to 26 September 2001 have non-zero [NODE,1] values (the low count nonlinearity was not well known at the time). If you have NICMOS data from Cycle 7 or 7N retrieved prior to this date and think that your data may benefit from the more accurate linearity corrections, you should reprocess the images (see Section 3.5), or retrieve them again using the OTFR.

1. The *correction* term in the nonlinearity equation given above is quadratic. This is then multiplied by the uncorrected flux, yielding an effectively cubic relation between uncorrected and corrected values.

BARSCORR (Bars Correction)

Some NICMOS images will have pairs of bright and dark columns or rows, which have come to be known as “bars”. The bars are believed to arise from electrical cross-talk in the detector lines during the readout of one camera when another of the cameras enters the auto-flush idle state. The bars manifest themselves as a noiseless DC offset of a few DN’s along a pair of columns or rows, with the pattern replicated exactly in all four image quadrants. They are discussed and illustrated in Section 4.3 of this *Handbook*.

Versions 3.3 and higher of **calnica** use the BARSCORR routine to remove the effects of the bars from MULTIACCUM observations. The routine scans pairs of columns or rows (depending on the camera) in each readout of the MULTIACCUM observation and identifies those with median signals more than 2σ different from the surrounding columns or rows as containing a bar. The user can set a different bars detection threshold by using the `barthresh` task parameter for **calnica**. It flags these pixels with a data quality value of 256 (bad pixel detected during calibration) in the DQ array of the appropriate imsets. In the subsequent CRIDCALC calibration step, where the data from all readouts is combined, the flagged pixels are rejected, so that the final combined image (*_cal.fits file) will be free of the bars.

No reference file is used by this step.



BARSCORR is available in version 3.3 and higher of calnica and all data retrieved from the HST Archive after 26 September 2001 are processed using the BARSCORR step. However, if you have Cycle 7 and 7N NICMOS data retrieved from the Archive prior this date and want to take advantage of this step, you will need to recalibrate your data, or to retrieve them again using the OTFR.

FLATCORR (Flat-Field Correction)

In this step the science data are corrected for variations in Detector Quantum Efficiency (DQE) between pixels by multiplying by an (inverse) flat-field reference image. This step is skipped for observations using a grism because the flat-field corrections are wavelength dependent. Starting with **calnica** version 4.4, this step uses the TDFFILE reference file, which contains the flat-field image for a given detector and filter (or polarizer) combination. The TDFFILE file contains five imsets, each with a flat-field image valid for a particular temperature range. Having a set of temperature dependent flat-fields makes it possible to correct for some of the temperature dependent pixel-to-pixel DQE variations seen in the NICMOS detectors. In the FLATCORR step, **calnica** reads the detector temperature from the TFBTEMP keyword and selects the appropriate imset from the TDFFILE to use. The particular imset used is written to the TDFGROUP keyword in the header of the calibrated *_cal.fits files. The temperature dependent flat-fields were delivered to the Archive on November 19, 2008 for Cycle 11 and later observations and on January 23, 2009 for data taken during Cycles 7 and 7N. For data retrieved prior to these dates there is no TDFFILE listed in the header. In this case, the FLATFILE reference file is used instead. This consists of a single static (non-temperature dependent) flat-field image. If both TDFFILE and FLATFILE reference files are given

in the header, **calnica** chooses the TDFFILE (unless the TFBTEMP keyword is missing, then FLATFILE is used instead). Error estimates and DQ flags contained in the TDFFILE/FLATFILE are propagated into the processed images.



*The difference between the temperature dependent TDFFILE and static FLATFILE flat-fields is small, but can affect the resulting photometry on a ~1% level. If you have retrieved images from the Archive prior to the dates given above, or have calibrated *_raw.fits images using calnica versions earlier than 4.4, and are concerned about photometry at a percent level, you may want to consider retrieving them again using the OTFR. You can also download the TDFFILES from the NICMOS Web page and rerun calnica (using a version 4.4 or later).*

UNITCORR (Convert to Count Rates)

The conversion from raw counts to count rates is performed by dividing the science (SCI) and error (ERR) image data by the exposure time (TIME) image data. No reference file is needed.

PHOTCALC (Photometric Calibration)

This step provides photometric calibration information by populating the photometry keywords PHOTMODE, PHOTFLAM, PHOTFNU, PHOTZPT, PHOTPLAM, and PHOTBW with values appropriate to the camera and filter combination used for the observation. The photometry parameters are read from the PHOTTAB reference file, which is a FITS binary table containing the parameters for all observation modes. The values of PHOTFLAM and PHOTFNU are useful for converting observed count rates to absolute fluxes in units of $\text{erg/s/cm}^2/\text{Angstrom}$ or Jy, respectively (see Section 5.2). PHOTTABs associated with NICMOS images retrieved after 23 January 2009 also include coefficients for correcting for the temperature dependence of the photometry caused by the temperature dependence of the DQE. **Calnica** (version 4.4 and later) reads the detector temperature from the TFBTEMP keyword and uses the coefficients to calculate a scaling factor that is stored in the ZPSCALE keyword of the *_cal.fits files. The output science image is then multiplied by this scaling factor to account for the temperature dependence of the DQE. The coefficients for Cycle 7 and 7N data are included in the PHOTTABs starting 23 January 2009. For Cycle 11 and later, the coefficients were updated in May 2009.



The photometry of NICMOS images may vary by up to a few percent due to variations in the detector temperature. If you are concerned about photometry at these levels and have data retrieved before the dates given above, you may want to download the images again using the OTFR. You can also download the PHOTABs from the NICMOS Web page and recalibrate using calnica (version 4.4 or later).

CRIDCALC Cosmic Ray Identification and Signal Accumulation)

This step identifies and flags pixels suspected of containing cosmic ray (CR) hits. For MULTIACCUM mode observations, this step also combines the data from all readouts into a single image. In MULTIACCUM mode, the data from all readouts are analyzed pixel-by-pixel, iteratively computing a linear fit to the accumulating counts-versus-exposure time relation and rejecting outliers from the fit as CR hits. The default rejection threshold is set to 4σ , but the user can override this, if desired, by setting the `crthresh` task parameter for **calnica**. The fit for each pixel is iterated until no new samples are rejected. Pixel samples identified as containing a CR hit are flagged in the DQ images of the intermediate MULTIACCUM (*_ima.fits) file, with a DQ value of 512. The pixel values in the SCI and ERR images of the *_ima file, however, are left unchanged.

Once all outliers have been identified, a final count rate value, and its uncertainty, are computed for each pixel using only non-flagged samples. The result of this operation is stored as a single imset in the output *_cal.fits file in which the number of unflagged samples used to compute the final value for each pixel and the total exposure time of those samples is reflected in the SAMP and TIME images, respectively. The variance ascribed to the final mean count rate is the uncertainty in the slope of the counts-versus-time relation at each pixel location, and is recorded in the ERR image of the *_cal.fits file. Pixels for which there are no unflagged samples, e.g., permanently hot or cold pixels, will have their output SCI, ERR, SAMP, and TIME values set to zero, with a DQ value that contains all flags that were set.

The CRIDCALC step also looks for curvature in the count vs. time relation. Such deviation from the expected almost linear response is rare but may occur close to bright or saturated sources, in particular in crowded fields. Pixels with curvature are assigned a flag value DQ=16384. This step is included in **calnica** version 4.2 and later. For more information see [ISR 2008-002](#). CRIDCALC is only applied to MULTIACCUM images. For data taken in ACCUM or BRIGHTOBJ mode, both the raw and calibrated images will contain cosmic rays and should be treated as with ordinary CCD data.

BACKCALC (Predict Background)

This step computes a predicted background (sky plus thermal) signal level, based on models of the zodiacal scattered light and the telescope plus instrument thermal background. This step uses the BACKTAB reference table which contains the background model parameters. Results of these predictions, along with direct estimates of the background level from the data themselves, are written to the BACKEST1, BACKEST2, and BACKEST3 header keywords. The image data are not modified in any way. **At the time of this writing, this step has not yet been implemented.** If there are future changes to the calibration procedures or software regarding the BACKCALC step, these will be reported in the *Space Telescope Analysis Newsletter (STAN)* and posted on the NICMOS Web site.

WARNCALC (User Warnings)

In this step various engineering keyword values from the *_spt.fits files are examined and warning messages are generated if there are any indications that the science data may be compromised due to unusual instrumental characteristics or behavior. **At the time of this writing, this step has not yet been implemented.** Any future changes to the software implementing WARNCALC will be reported in the *Space Telescope Analysis Newsletter (STAN)* and posted on the NICMOS Web site.

3.3.3 Runcalsaa

The **runcalsaa** routine in the pipeline comprises of two **PyRAF** tasks, **saaclean** and **nic_rem_persist** which are available in the **stdas.hst_calib.nicmos** package. **Runcalsaa** removes persistence from images affected by SAA passages as well as Bright Earth Persistence which are discussed below. **Runcalsaa** runs on cal images which are output of calnica. **Saaclean** is run only when the SAA_DARK and FLATFILE keywords are populated in the raw file header.

SAACLEAN: Removing SAA Persistence from NICMOS Images

Approximately half of all HST orbits transit through the South Atlantic Anomaly (SAA), where the cosmic ray rate is so high that their residual flux contributes a significant noise component to many subsequent exposures. NICMOS data is particularly susceptible to this "image persistence" or latent charge. This residual charge escapes slowly, introducing a decaying "persistence" in potentially many science exposures during the same orbit. For more details about SAA persistence please refer to Section 4.8.2.

In an attempt to recover the lost signal-to-noise in the SAA-impacted science exposures, a **PyRAF** task called **saaclean** was developed (see NICMOS [ISR 2007-001](#)) and has been implemented in the OTFR pipeline.

This task is run on post-SAA NICMOS images to identify the amount of charge in each pixel that can be attributed to persistent flux from SAA cosmic rays, and apply a correction based on an SAA persistence model to remove this flux from the data.

The **saaclean** task will be run on science data in the pipeline only if the data is determined to be SAA-impacted. If the task determines that the science data signal-to-noise would be improved with a correction, the task will apply the correction to the *_cal.fits file and populate the associated keywords in the science exposure header. Please see the **saaclean** task help file in the **stdas.hst_calib.nicmos** package of **PyRAF** and the NICMOS [ISR 2007-001](#) for more complete details.

NIC_REM_PERSIST: Removing Bright Earth Persistence from NICMOS images

It has recently been found that the NICMOS detectors may be exposed to another type of persistence, Bright Earth Persistence (BEP, see Section 4.8.3) This occurs in rare instances when HST is pointed towards the bright earth and one or more of the NICMOS filter wheels are not yet in the blank position.

Removal of the BEP is done in a manner similar to the removal of cosmic ray induced persistence from SAA passages. A stored BEP persistence image is scaled to the measured persistence and subtracted from the science image. This procedure is repeated until less than 50% of the background pixels are affected. This rather high limit is set to avoid affecting sources in the image. Due to the large coverage of afflicted pixels, the scaling is done by minimizing the residuals relative to a flat sky (without sources). In contrast, SAA cosmic ray persistence is scaled by minimizing residuals relative to adjacent pixels.

A number of new keywords are introduced to handle the BEP removal. The task **nic_rem_persist** uses persistence model file given by the keyword **PMODFILE**, and persistence mask file given by the keyword **PMSKFILE**. Both these reference files are specific for each camera. Calibration indicator **BEPDONE** indicates whether the BEP correction was applied or not. Bright Earth Persistence keyword **BEPSCALE** shows the level of persistence calculated, a default value of **BEPVALLO=0.5** shows minimum allowed value of the persistence to apply, a default value of **BEPUSELO=0.5** shows minimum allowed fraction of pixels used and **BEPFRAC** gives the fraction of pixels used to calculate persistence.

Please note that the BEP removal procedure has been implemented in the pipeline for NIC2(2008) and it will soon be implemented for NIC1 and NIC3. Check the [NICMOS Web](#) page for updates.

3.4 Mosaicing/Drizzling

Calnicb was NICMOS's initial standard method of combining exposures to create mosaiced images. During this period **calnicb** was incorporated into the OPUS pipeline and recommended to users for use on their local machines. However, **calnicb** does not correct for the geometric distortion present in NICMOS images, which is small but can be important for some applications (see Section 5.3 for a discussion). Due to this shortcoming **calnicb** is no longer the recommended software for creating NICMOS mosaic images. We now recommend the **MultiDrizzle** software package which can be run in **PyRAF** and includes a geometric distortion correction.

In the following subsections we provide an overview of the **MultiDrizzle** task and **calnicb**. Even though we no longer recommend the use of **calnicb** by users on their local machines the software is still present in the OPUS pipeline and so the user may still come across **calnicb** outputs while working with NICMOS data. For this and historical reasons we include a brief overview of the **calnicb** algorithm but still recommend **MultiDrizzle** for all NICMOS mosaicing applications.

3.4.1 MultiDrizzle

At the time of writing of this handbook, the preferred method to combine and mosaic NICMOS observation is to use the **MultiDrizzle** routine in the **stsdas.analysis.dither** package. The latest version of this routine now fully support NICMOS data and allows for users to optimally mosaic their data using the drizzle algorithm. **MultiDrizzle** can be used to both create a combined mosaic of the available data, further refine the rejection of cosmic rays, and produce images with optimally resampled pixel size to make full use of all the information contained in original dithered data. A full description of how to run **MultiDrizzle** with NICMOS data is available in the NICMOS section (Section 6.3) of the **MultiDrizzle** Handbook at:

http://www.stsci.edu/hst/HST_overview/documents/multidrizzle

3.4.2 Calnicb

The **calnicb** task produces the combined, or *mosaiced*, image from the multiple images contained in a NICMOS association. The task also performs background subtraction and source identification on the images in the association. It was designed to implement the potentially complex task of image mosaicing in a pipeline fashion, but sometimes a more careful, manual treatment can be worthwhile. As mentioned earlier **calnicb** does not include any correction for geometric distortion in NICMOS

images, nor does it allow pixel subsampling which may be useful in order to improve image resolution for undersampled images (especially with NIC3). Also, some NICMOS users dithered their observations “manually” using POS-TARG offsets rather than the canned patterns available in Phase II; such data sets will not be linked as associations in the *HST* archive. Finally, you may wish to have more interactive control over the various stages of the background subtraction, registration, and coaddition process than **calnicb** offers. For all these reasons we recommend that the user employ the **MultiDrizzle** task.

Input Files

Three pieces of input data are needed by **calnicb**:

1. The *association table* (*assoc_id_asn.fits*): this is a table containing the list of members in the association and relevant information on the association type, as given in Table 3.1

Table 3.1: Columns of the Association Table (input to calnicb)

Column Name	Meaning
MEMNAME	Rootname (<i>IPPPSSOOT</i>) of each image in the association.
MEMTYPE	Role or type of each member: EXP-TARG = input exposure for target EXP-BCK _{<i>n</i>} = input exposure of <i>n</i> ’th background (for chop patterns) PROD-TARG = output product containing target PROD-BCK _{<i>n</i>} = output product containing <i>n</i> ’th background (for chop patterns)
MEMPRSNT	Flag indicating whether or not a member is present (needed by the STScI automatic pipeline processing).

The table extension header of the *assoc_id_asn.fits* file also contains the keywords which control the background illumination pattern correction (ILLMCORR). The keywords used are: ILLMCORR (whether or not the correction is to be performed) and ILLMFILE (reference file name for the illumination correction). These are further discussed later in this Section.

2. The input calibrated images (*ippssoot_cal.fits*): the science data images which are part of the association, as listed in the first column of the association table. The images are usually the calibrated outputs of **calnica**.
3. The support files (*ippssoot_spt.fits*), containing engineering information, so that **calnicb** can transfer this information to the output support files.

Output Files

Calnicb produces three types of output:

1. An updated copy of the association table (*assoc_id_asc.fits*): this copy of the *assoc_id_asn.fits* file contains additional information about the processing that took place. The *assoc_id_asc.fits* file contains four additional columns, listed in Table 3.2

Table 3.2: Additional Columns of the Output Association Table

Column Name	Meaning
BCKIMAGE	Flag indicating whether or not the image was used to compute the background.
MEANBCK	Values of the mean background for the image (DN/sec).
XOFFSET	X-offset (in pixels) of the image from the reference frame; a positive value means a positive offset of the image (not of the sources) relative to the reference.
YOFFSET	Y-offset (in pixels) of the image from the reference frame; a positive value means a positive offset of the image (not of the sources) relative to the reference.

Additional information contained in the header of the *assoc_id_asc.fits* table is the `MEAN_BKG` keyword, which gives the constant background signal level subtracted from all images in the association.

2. One or more output mosaic images (*assoc_idn_mos.fits*): the number of output mosaic images depends on the pattern. The target field is always contained in the *assoc_id0_mos.fits* file. Patterns which involve chopping onto the sky to produce background reference images result in multiple *assoc_idn_mos.fits* files after processing through **calnicb**, with the background positions identified by $n=1$ to 8.
3. One *assoc_idn_spt.fits* support file for each *assoc_idn_mos.fits* file created.

Processing

The basic philosophy of the **calnicb** algorithm is to remove the background from each image after source identification, to align the images by calculating offsets, and to produce the final mosaic. The processing steps of **calnicb** can be summarized as follows:

1. Read the input *asn* table and input images.
2. Determine processing parameters from keyword values.
3. Combine multiple images at individual pattern positions.

4. Identify sources in the images.
5. Estimate and remove the background signal.
6. Create a mosaic image from all pattern positions.
7. Write the output association table and mosaic images.

The sections below discuss steps 2 through 6 in greater detail.

Processing Parameters

Header keywords from the input `*_cal.fits` images are read and evaluated in order to guide the **calnicb** processing. One set of keywords (Table 3.3) pertains to the association as a whole and therefore are read only once from the first input member image:

Table 3.3: Keywords Common to all Datasets in an Association

Keyword	Purpose
INSTRUME	Check whether they are NICMOS data.
CAMERA	Camera number.
FILTER	Filter name; if set to “BLANK”, the association is made of darks.
IMAGETYP	Type of image (EXT=external, DARK=dark frames, FLAT=flat-field images).
NUMITER	Number of iterations for each exposure.
PATTERN	Pattern used.
NUMPOS	Number of independent positions in the pattern.

A second set of header keywords (Table 3.4) are specific to each member of the association, and must be read from each input image.

Table 3.4: Dataset-specific Keywords

Keyword	Purpose
PATT_POS	Position of the image in the pattern.
BACKEST n	Background estimates from calnica .
CRPIX n , CRVAL n , CD n_n , CTYPE n	World Coordinate System (WCS) information (see Table 2.4).

Based on this information, an inventory is taken of which input images exist, where they belong in the pattern, how many images there are at each pattern position, which images belong to the target field, which ones are from background fields, and to which output mosaic image each input image will contribute. As part of the input process, the appropriate

ILLMFILE reference file is loaded. Note, however, that the ILLMFILES used in this step are dummies, and have no effect on the data. In fact, the ILLMFILES provided by STScI have their PEDIGREE set to DUMMY, thus forcing the stage to be skipped. The ILLMFILES were introduced to remove a two-dimensional residual background that may exist due to spatial variations in the thermal emission of the telescope and instrument. However, in practice, it does not appear that there are strong spatial illumination variations requiring such corrections, and therefore the ILLMFILES used in the processing pipeline are dummies. These files *must* be present, however, in order for **calnick** processing to proceed. The step may also be turned off entirely by setting ILLMCORR to OMIT in the association table (by default, it is set to PERFORM, even though dummy files are used). In order to disable ILLMCORR, the keyword must be changed in the association table header itself, *not* in the primary image header of the association table FITS file. This must be done with the **tables.parkey** task, not with **hedit**. See the highlighted note at the end of Section 3.5.2 for how to do this. Ordinarily, it is simplest to just leave ILLMCORR=PERFORM and use the dummy reference files.

Combination of Multiple Exposures

If there is more than one image at any pattern position ($\text{NUMITER} > 1$), the multiple images at each position are first registered and then combined into a single image. The coordinates (as determined by the WCS keywords) of the first image at a given pattern position are used as a reference for the registration. The offsets to all other images at that pattern position are first computed by comparing their WCS data, and then refined using a *cross-correlation* technique, down to a level of 0.15 pixels. The cross-correlation technique employs an algorithm which minimizes the differences between fluxes in the images. The computed offsets, in units of pixels, are recorded in the output association table. After determining the relative offsets, the images are aligned using *bilinear interpolation* and are then combined on a pixel-by-pixel basis. The combined pixel values are computed as a weighted mean of all unflagged (i.e., $\text{DQ} = 0$) samples, using the input image ERR values as weights. If three or more samples are present, iterative σ -clipping is performed to reject outliers. The number of samples used at each pixel and the total integration time are retained.

Source Identification

The source identification step is used for excluding sources when the background in the images at each pattern position is estimated. The images at each pattern position are searched for pixels suspected to contain signal from a source. The median signal level in the image is computed and pixels that are more than 4.5σ above the median are considered as candidates. Spurious results, such as pixels containing cosmic-ray hits, are filtered out by searching neighboring pixels and only retaining those candidates that have two or more neighbors that are also above the threshold. The DQ flag of the source-affected pixels is then set to 1024.

Background Estimation and Removal

A *constant background* signal level, which is estimated from the images themselves is removed from the images at each pattern position as follows.

1. With chop patterns, the median and average deviation of the signal in the image at each chop position is computed. In addition to excluding bad and source-flagged pixels, the calculation of the median also uses iterative sigma-clipping to reject outliers.
2. With dither-only patterns, or with multiple-exposure single pointings, the median and average deviation of each target image is computed. The result for each image is compared to the background estimate provided by **calnica**, which is (in principle) stored in the BACKEST1 header keyword of each image. The value computed by **calnicb** is accepted if it is less than 5σ deviant from that of **calnica**, otherwise the **calnicb** value is assumed to be biased by the presence of sources and the **calnica** value is substituted for it. Note, however, that normally the value of BACKEST1 would be populated by the BACK-CALC step of **calnica**, which has not been implemented (see Section 3.3.2). Therefore ordinarily BACKEST1 has value 0.0, and in this case the background value computed by **calnicb** is always used, unless the user has manually set BACKEST1 to some non-zero value.
3. The global constant background signal is computed by taking the mean of the background values for each image, again, using iterative sigma-clipping to reject outliers.
4. The final mean background value is subtracted from all images (both target and background images, if present).
5. With dither-only patterns, the user has the option of subtracting the individual background values computed for each image from themselves rather than computing and subtracting a global mean background value. This option is controlled by the `meanbkg` task parameter for **calnicb**. The default value, “yes”, indicates that the global mean is to be used.

Mosaic Construction

Mosaic (MOS) images are created for each independent pointing within the pattern. For example, a combination DITHER-CHOP pattern will produce one mosaic image out of the dithered pattern at each CHOP location on the sky. Each mosaic image is created as follows:

1. The relative offsets between images within the mosaic are computed from their WCS information and refined using cross-correlation (as in the case of multiple exposures at each pattern position; see “Combination of Multiple Exposures” on page 60). The first image in the list for each mosaic is used as a reference image.
2. An empty mosaic image is created with x and y dimensions large enough to encompass the maximum offsets in each direction.

3. Pixel values in the mosaic image are populated by combining samples from overlapping images. The individual images are aligned using bilinear interpolation and the value at a given mosaic pixel location is computed from the error-weighted mean of the samples at that location. Samples flagged as bad are excluded and, if three or more samples are present, iterative sigma-clipping is used to reject remaining outliers. The number of samples retained for a given pixel and their total integration time is recorded in the SAMP and TIME images, respectively. If all samples are rejected for a pixel, the mosaic image SCI, ERR, SAMP, and TIME values are set to zero and a combination of all DQ flags is retained.

3.5 Recalibration

This section is intended to help you decide whether your data were calibrated with optimal calibration reference files and to help you decide whether you need to recalibrate your data.

3.5.1 Why Recalibrate?

In many cases, NICMOS calibrated data produced by the OPUS pipeline—the standard calibration—are adequate for scientific applications. However, as with all instruments, there is often room for improvement, and you may find it worthwhile or even necessary to reprocess your data, perhaps following additional procedures which are not part of the standard pipeline. As described at the start of this chapter, Cycle 7 and 7N data delivered to the observer or retrieved from the *HST* archive before 26 September 2001 were calibrated with the best, instrument configuration-specific reference files available at the time of the observation. However, updated or timely reference files sometimes do become available after the data were taken and first processed. As one important example, the DARK reference files were substantially updated and improved during and after Cycle 7. Also, after the installation of NCS, new sets of darks and flat fields were needed as a consequence of the higher operational temperature. Improved software for calibration (updates to **calnica**, as well as new tasks external to the standard pipeline, such as **MultiDrizzle**) has become available as our understanding of the instrument performance has increased with experience. For example, the ZSIGCORR step of **calnica** was added during Cycle 7, and BARSCORR was implemented in **calnica** version 3.3. As an example of a more recent change, the pipeline was updated in 2008-2009 to account for the temperature dependence of the dark and flat-field reference files as well as the temperature dependence of the photometry.

After 26 September 2001, NICMOS data retrieved from the Archive are automatically reprocessed by OTFR using the latest pipeline software and calibration reference files. Therefore if you have data retrieved prior to important updates in the pipeline, the easiest way to recalibrate is to retrieve the data again using the OTFR. However, there are still situations where you may wish to reprocess your data locally, using non-standard reference files or software tools. For example, reprocessing may be necessary to correct the NICMOS bias.

Moreover, NICMOS data are subject to a variety of anomalies which may complicate the task of data reduction. These are discussed extensively in Chapter 4. In many cases, procedures and software for handling these anomalies were not available when the observations were made or retrieved from the Archive. If you notice unusual features in your data (see, e.g., the checklist at the start of Chapter 4), or if your analysis requires a high level of accuracy, you may wish to explore whether a better set of calibration reference files exist than those that were used to process your data, or if additional processing steps may be needed. If better files are available or the calibration software has changed significantly, you may choose to recalibrate your data using the new files or software.

Finding that a calibration reference file has changed since your data were calibrated doesn't always mean that you have to recalibrate. The decision depends very much on which calibration image or table has changed, and whether that kind of change to your data is likely to affect your analysis in a significant way. Before deciding to recalibrate, you might want to retrieve the new recommended reference file or table and compare it to the one used to calibrate your data at STScI in order to determine if the differences are important. You can use the table tools in the **IRAF ttools** package to manipulate and examine calibration tables. Reference files can be manipulated in the same way as your science data.

Finally, the observations may have been made in a non-standard way. Some of the input files (e.g. *_asn.fits) may require manual editing before recalibration.

3.5.2 Recalibrating the Data

This section describes the mechanics involved in actually recalibrating a dataset. As noted above, the simplest way to recalibrate your data is to retrieve it again from the *HST* Archive using OTFR. However, it is sometimes more convenient to simply reprocess your raw data locally using the latest pipeline software or reference files. In some cases, when you may wish to use special, customized reference files or processing software, local reprocessing is your only option.

The basic steps in recalibrating a dataset on your own computer are:

1. Assemble any necessary reference files or tables and your raw data files.

2. Set the desired calibration switches and reference file name keywords in the *primary header* of your raw (`*_raw.fits`) data file. These determine which steps will be executed by the calibration software and which reference files will be used to calibrate the data.
3. Run the calibration software.

Assembling the Input Files

In order to recalibrate your data, you need to retrieve *all* of the reference files and tables that are used by the calibration steps you want to perform. The source of these files is the Calibration Database (CDBS) at STScI. A complete description of how to retrieve the reference files is given in Chapter 1 of the "[HST Data Handbook](#)".

Setting the Calibration Parameters

The calibration software is completely data-driven, meaning that the calibration steps to be carried out are determined by the values of the *calibration switches* and the *calibration reference files* keywords contained in the primary header of the file to be processed. An important step is then to set the calibration switches and reference file keywords in the primary header of your raw data file (`*_raw.fits`) to reflect how you want the data recalibrated and which reference files you want to use at each step in the process. This is done most easily with the **chcalpar** task in the **hst_calib.ctools** package of STSDAS or with the **hedit** task in the **IRAF images** package.



The calibration switch keywords reside only in the primary header of NICMOS FITS files. Therefore it is critically important to specify extension number zero when passing file names to tasks like hedit to modify these keywords. For example, to modify calibration keywords in the file `n3xe01bhm_raw.fits`, be sure to use the name `n3xe01bhm_raw.fits[0]` as input. If you specify any other extension number, the keywords you modify will end up getting written into the header of that extension instead, where calnica will not find them.

The **chcalpar** task takes a single input parameter—the name(s) of the raw data files to be edited. When you start **chcalpar**, the task automatically determines that the image data are from NICMOS and opens a NICMOS-specific parameter set (*pset*) that will load the current values of all the calibration-related keywords. To edit the calibration keyword values:

1. Start the **chcalpar** task, specifying the image(s) in which you want to change keyword values. Note that with **chcalpar**, it is not necessary

to append the primary header extension [0] to the image name. If you specify more than one image, for example using wild cards, the task will read the initial keyword values from the first image in the list. For example, you could change keywords for all NICMOS raw science images in the current directory (with initial values from the first image), using the command:

```
ct> chcalpar n*raw.fits
```

2. After starting **chcalpar**, you will be placed in **eparam** [the **IRAF** parameter editor], and will be able to edit the set of calibration keywords. Change the values of any calibration switches, reference files or tables to the values you wish to use for recalibrating your data.

Exit the editor when you are done making changes by typing:q two times. The task will ask if you wish to accept the current settings. If you type “y”, the settings will be saved and you will return to the **IRAF** c1 prompt. If you type “n”, you will be placed back in the parameter editor to redefine the settings. If you type “a”, the task will abort and any changes will be discarded.



*As delivered from the archive, image header parameters which specify the names of the calibration reference files (e.g, **FLATFILE**, **DARK-FILE**, etc.) take the form **nref\$name_ext.fits** or **ntab\$name_ext.fits**. The prefixes **nref\$** and **ntab\$** are environment variables pointing to the **CDBS** directories where the reference files reside at STScI. This can be convenient, and you may wish to keep your calibration reference files in a particular directory when reprocessing your data. However, because **calnica** is a stand-alone C program called by **IRAF**, the environment variables **nref** and **ntab** must be defined at the system host level, before starting an **IRAF** session. For **UNIX** environments, this is done with **setenv nref /path/** and **setenv ntab /path/**, where you should specify the path to your reference file directory. Do not forget the trailing slash!*

Running the Calibration Software

After you change the header keyword values for your raw data files, you are ready to recalibrate your data. To run **calnica**, type the name of the task followed by the names of the input raw data file and desired output

calibrated data file. For example, to recalibrate the dataset n0g70106t, you could type:

```
ni> calnica n0g70106t_raw.fits n0g70106t_cal.fits
```

or simply:

```
ni> calnica n0g70106t ""
```

To run **calnicb** the name of the association table must be given as input:

```
ni> calnicb assoc_id_asn
```

To run **calnicb** on a subset of the *_cal.fits files, it is sufficient to edit the *_asn.fits table and remove the undesired files.



The calibration routines calnica and calnicb will not overwrite an existing output file. If the calibration tasks are run in the directory where the original calibrated files are located, a different output file name must be specified.



*There are some calnicb processing parameters which reside in the association (*_asn.fits[1]) table header and not in any FITS file image header, and which therefore cannot be changed using chcalpar or hedit. In particular, to change the ILLMCORR and ILLMFILE parameters, you must use the parkey task on the *_asn.fits[1] file. As an example, to change the ILLMFILE, type: parkey /path/name_ilm.fits data_asn.fits[1] ILLMFILE, where /path/name_ilm.fits is the full name and path to the ILLMFILE, and data_asn.fits is the association table you are editing. In order to set ILLMCORR to OMIT and skip this processing step entirely, type: parkey OMIT data_asn.fits[1] ILLMCORR.*

3.6 Calibration Goals and Plans

This chapter describes the calibration accuracies that we aim to reach in Cycle 17. Since the NCS-operated NICMOS represents a new instrument, a full suite of calibrations have been carried out since the installation of the NCS through Cycle 16 to characterize the instrument performance under the new operation conditions. The plans and goals for Cycle 17 are described in this chapter.

3.6.1 Calibration Accuracies

In Table 3.5 we summarize the calibration goals for Cycle 17, assuming a 12 month duration of cycle. Observers with science programs that require better calibrations should request and justify additional observing time for any supplemental calibrations necessary to achieve their goals.

The calibration proposals that have been executed during the SMOV phase, as well as the ones included in Cycle 10 through 16, have been aimed at reproducing and possibly improving the level of calibration accuracy achieved during Cycle 7 and 7N. As discussed in Section 3.3.1, the temperature of the NICMOS detectors, as measured by the temp-from-bias method, has shown a drift since Cycle 11. The temperature decreased by $\Delta T \sim 2\text{K}$ during the period 2002 to 2008. Using the calibration programs from Cycle 11 to 16, the NICMOS team has been able to quantify the effects from this temperature drift on the calibration of the detectors. As a result, new temperature dependent reference files are now available. To continue the investigation of this temperature dependence, as well as the overall detector performances, the monitoring programs continue in Cycle 17.

3.6.2 Monitoring Programs

As shown in Table 3.5, several programs aim at routinely monitoring the proper operation of NICMOS. Programs to routinely obtained darks, and determine the shading profile of the detectors (11946, 11947), monitor the stability of the flat-fielding in a few broad filters (11948), monitor the photometric stability of the instrument (11950), and to monitor (and correct if necessary) the focus settings of the instrument (11953) are planned. These programs, and the accuracies aimed by these programs are listed in Table 3.5

Table 3.5: NICMOS CYCLE 17 Calibration Plan

ID	Proposal Title	PI	Frequency	Time (orbits)		Scheduling Required	Accuracy Required	Notes
				External	Internal			
Routine monitoring programs								
11946	Dark Current and Shading Profile	Dahlen	1/month		12	Throughout cycle	4-5% per visit for lin. dark, S/N 50 overall	Routine monitor of dark current and shading profile for all 3 cameras.
11947	Extended Dark Monitoring	Dahlen	Bi-monthly		120	Throughout cycle	5%	Extended dark, amplifier and shading, for all 3 cameras, incl temp dependence.
11948	Flats Stability	Dahlen	1 orbit ~6 months	2		Throughout cycle	1-2%	Monitor DQE change with temperature/time for all 3 cameras.
11950	Photometry Monitoring	de Jong	1 orbit ~4 months	3		Throughout cycle	1-2%	Verify photometry stability over a wide range of wavelengths.
11953	Focus Monitoring	Wiklind	Every ~4 months	7		Throughout cycle	1mm	Monitor focus of all 3 cameras.
Special closeout/legacy programs								
11949	Temperature-dependent flat fields	Dahlen	1/year	8		Throughout cycle	1-2%	Calibrate time/temperature dependence of flat-fields for a range of filters
11951	Calibrating NICMOS Non-linearity in F160W	de Jong	1/year	9		Mid-cycle	1-2%	Calibrate non-linearity at very faint levels at long wavelengths
11954	Photometric Cross-Calibration	Bohlin	1/year	8		Throughout	1-2%	Observe faint IR spectrophotometric standards
SMOV4 Carry-over programs								
11952	Photometric Standards Imaging	de Jong	1/year	6		Early in cycle	1-2%	Post-SM4 photometric calibration
11955	Grism Calibration	Pirzkal	once	3		Early in cycle	2%	Post-SM4 grism calibration
TOTAL NUMBER OF ORBITS				46	132			

3.6.3 Special/Legacy Programs

Cycle 17 includes three special calibration programs that are not part of the standard monitoring. First, program 11949 will obtain flat-fields for a range of different filters in order to characterize the flat-field behavior at the detector temperature valid for Cycle 17. Program 11951 will extend the flux-dependent non-linearity calibration to fainter limits than previously measured, in order to enable non-linearity corrections to be applied to observations of faint, distant sources. This proposal uses the F160W filter, and is complementary to the Cycle 16 F110W proposal 11799. The purpose of the third special program 11954 is to provide improved spectrophotometric observations for faint IR standards to be used in cross-calibrating to WFC3/IR and JWST.

3.6.4 SMOV Carry-over programs

Two programs in Cycle 17 are intended to verify the behavior of the NICMOS detectors after Servicing Mission 4. This includes observing standard stars to verify the photometric calibration (11952) as well as the calibration of the NICMOS camera 3 grisms (11955).

Further details about these proposals can be obtained from:

<http://www.stsci.edu/hst/>

3.6.5 Calibration in Previous Cycles

Information about the calibration plans for Cycles 10-15 can be obtained in [ISR 2002-002b](#), [ISR 2002-03](#), [ISR 2003-11](#), [ISR 2005-005](#) and [ISR 2007-004](#). These can be found at:

<http://www.stsci.edu/hst/nicmos/documents/isrs/>

3.6.6 Special Calibrations

If your program requires unique calibrations beyond those that are planned and listed in Table 3.5, then you should apply directly for these special calibrations in your Phase I proposal.

Anomalies and Error Sources

In this chapter. . .

4.1 NICMOS Problems Checklist / 71
4.2 NICMOS Dark Current and Bias / 73
4.3 Bars / 91
4.4 Detector Nonlinearity Issues / 93
4.5 Count Rate Non-Linearity / 96
4.6 Flat Fielding / 98
4.7 Pixel Defects and Bad Imaging Regions / 101
4.8 Effects of Overexposure / 105
4.9 Cosmic Rays of Unusual Size / 113
4.10 Scattered Earthlight / 115

4.1 NICMOS Problems Checklist

NICMOS data are subject to a variety of anomalies, artifacts, and instabilities which complicate the task of data reduction and analysis. Most of these can be handled with careful recalibration and processing, which usually yields excellent, scientific grade data. Careful NICMOS data processing usually requires a certain amount of “hands-on” interaction from the user, who must inspect for data anomalies and treat them accordingly during the reduction procedures. In some cases, recognizing and treating problems with NICMOS data requires a moderately in-depth understanding of the details of instrumental behavior; problems with dark and bias subtraction are good examples

We begin with a checklist of potential NICMOS instrumental anomalies and potential data processing problems about which the user should be

aware. Each of these is discussed in further detail in the sections which follow: the nature of the problem and its impact on NICMOS data is illustrated, and possible processing solutions are considered. The relevant sections for each anomaly are given in parentheses below.

NICMOS Problems to Watch Out For: A Checklist

- Bias and dark subtraction problems, including:
 - residual shading (Section 4.2.2, Section 4.2.4)
 - variable quadrant bias or “pedestal” (Section 4.2.2, Section 4.2.4)
 - bias jumps or bands (Section 4.2.2, Section 4.2.4)
- Bars (Section 4.3)
- Nonlinearity correction uncertainties
 - nonlinearity corrections (Section 4.4.1)
 - non-zero zeroth read correction (Section 4.4.2)
 - uncorrected saturation (Section 4.4.3)
- Count rate non-Linearity (Section 4.5)
- Flat-field issues, including color dependent flat fields (Section 4.6)
- Pixel defects and bad imaging regions, including:
 - Hot pixels, Cold pixels and Grot (Section 4.7.1)
 - Erratic middle column/row (Section 4.7.2)
 - Coronagraphic hole masking (Section 4.7.3)
 - Vignetting (Section 4.7.4)
- Effects from bright targets:
 - Photon-induced persistence (Section 4.8.1)
 - Post-SAA cosmic ray persistence (Section 4.8.2)
 - Bright Earth Persistence (Section 4.8.3)
 - The “Mr. Staypuft” Effect (amplifier ringing) (Section 4.8.4)
 - Optical ghosts (Section 4.8.5)
- Cosmic rays of unusual size (Section 4.9)
- Scattered earthlight (Section 4.10)

4.2 NICMOS Dark Current and Bias

Some of the major challenges for achieving high quality NICMOS data reduction arise from difficulties in removing additive components of the instrumental signature that are present in a raw NICMOS image. For the purpose of discussion here, we will divide these additive components into two categories, bias and dark, according to whether or not the signal is noiseless and purely electronic in origin (bias), or noisy and arising from thermal or luminous sources (dark). In practice, the NICMOS bias and dark signals each consist of several different components which exhibit a range of different behaviors.

In the past, the reference files used for processing NICMOS data, had the dark and bias components combined together to a single dark image that was used in the DARKCORR step of the calnica pipeline processing. NICMOS dark images (really dark + bias) are highly dependent on the readout history of the array since it was last reset, and therefore cannot be simply rescaled to the exposure time of the science data (as is done with most conventional CCD data). Each science file must be calibrated with a dark frame of equal exposure time and number of readouts.

Such "composite" dark calibration reference files for all MULTIACCUM readout sequences have been constructed using as basic data the on-orbit darks obtained from calibration (dark monitor) programs. The filenames of the "composite" darks are written to the DARKFILE header keyword. These composite darks have now been superseded by newly created temperature-dependent dark calibration reference files (see Section 4.2.3 for more details). The file names of these "*_tdd" files are written to the TEMPFILE header keyword. If both the TEMPFILE and DARKFILE keywords are populated, the former will be used.

Unfortunately, some components of the NICMOS bias and dark have turned out to be unstable or unpredictable, making it difficult or impossible to remove them using the standard reference files. In order to do a good job removing additive dark and bias signatures, it is important to understand their origin and behavior. Here we describe the various components of NICMOS biases and darks in some detail, highlighting their stability or lack thereof, and describing (briefly) how they are incorporated into the standard STScI dark reference images. In Section 4.2.4 below we describe methods and tools for measuring and removing residual dark and bias artifacts from NICMOS images.

4.2.1 Dark Current


Linear Dark Current

The true, thermal dark current is the detector current when no external signal is present. This component grows linearly with integration time:

$$D(x,y,t) = dc(x,y) \times t$$

where $D(x,y,t)$ is the observed signal in a given readout, t is time since reset, and $dc(x,y)$ is the dark current count rate. At the operating temperatures used for NICMOS in Cycle 7, the mean dark current for all three cameras was of order 0.1 e⁻/sec. In Cycle 11, when operating at warmer temperatures with the NCS, the dark current has some two dimensional structure, and is roughly a factor of two higher in the corners than at the center. At the higher temperature, the dark current has a “salty” appearance due to a large number of high countrate pixels. In addition, particularly in NIC3, there are large areas of higher dark current across the chip. (See Figure 4.1).

Figure 4.1: Dark Current Comparison Between Cycle 7 and Cycle 11.

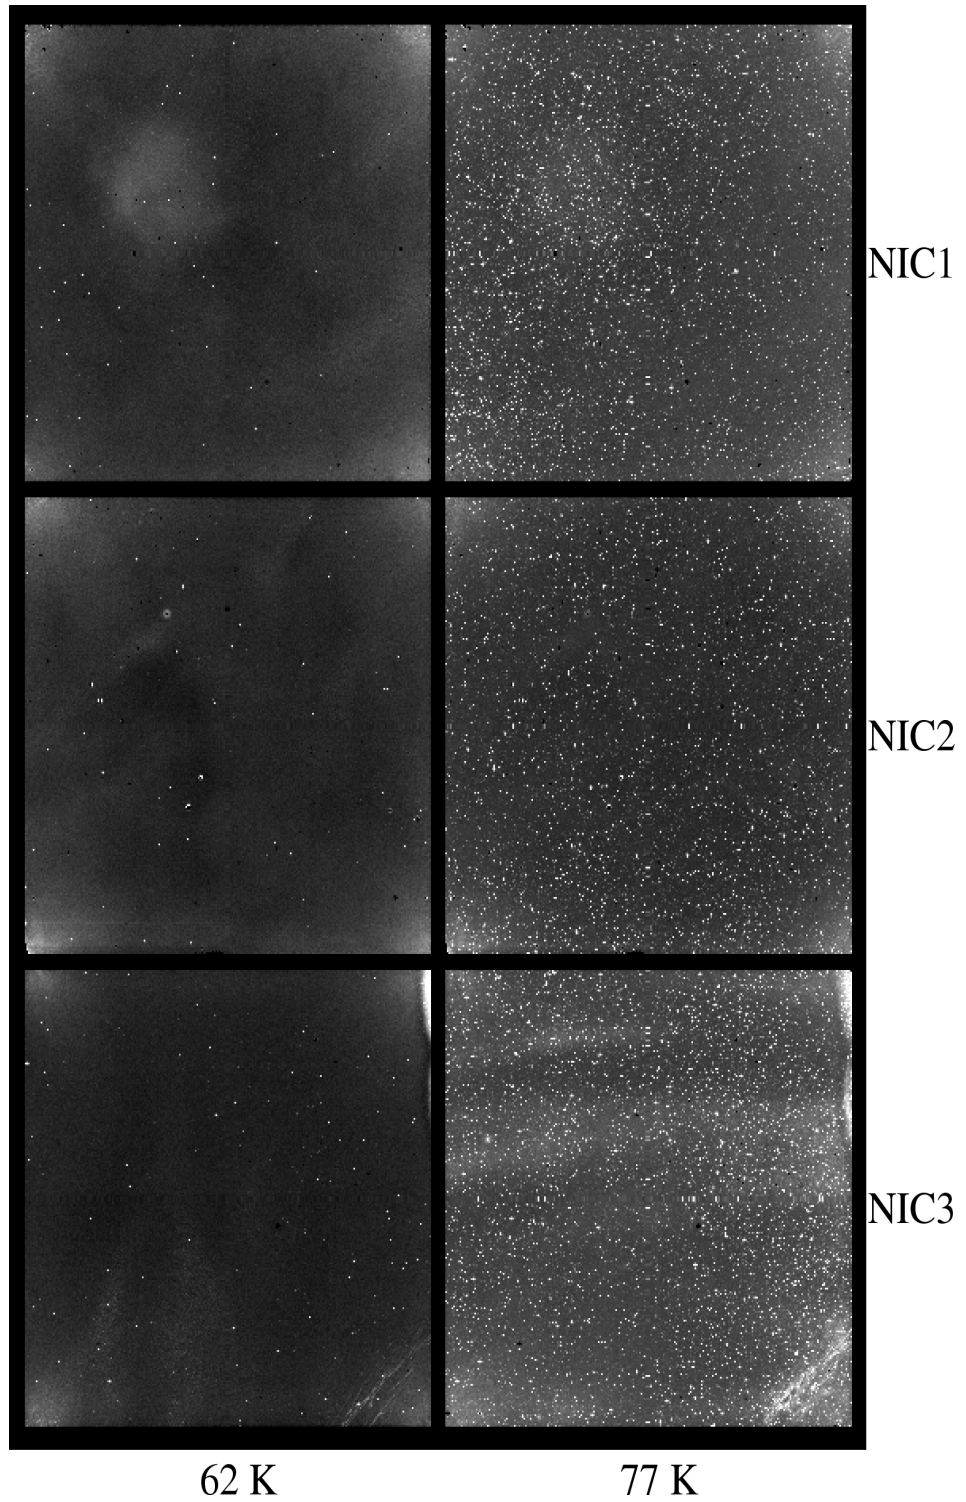

Amplifier Glow


Each quadrant of a NICMOS detector has its own readout amplifier, which is situated close to an exterior corner of the detector. When a readout is made, the amplifier emits radiation which is recorded by the detector, an effect known as amplifier glow (Figure 4.2). This signal is largest close to the corners of the detector where the amplifiers are situated, and falls off rapidly towards the center of the array. The signal is only present during a readout while the readout amplifiers are powered, but is repeated for each readout (e.g., a MULTIACCUM sequence or an ACCUM with multiple initial and final reads). Typically the extra signal is about 20-30 DN at the corners of the detector and 2-3 DN at the center, for each readout. The signal is highly repeatable, and linearly dependent on the number of reads. This is also dependent on temperature. The amplifier glow also depends on the length of time for which the amplifiers are switched on, which is slightly shorter (by ~14%) for ACCUM mode.

The amplifier glow is a real, detected signal and is subject to photon statistics, so it is a source of noise in NICMOS exposures. In the processing pipeline and calibration reference files, it is considered to be a component of the dark signal, although its physical origin and temporal dependence is quite different than that of the thermal dark current. Thanks to the repeatability of the signal, images calibrated with the appropriate dark frames (same MULTIACCUM sequence or same exposure time for ACCUM images) will have the amplifier glow removed in the DARKCORR step in **calnica**. This component grows with number of readouts:

$$A(x,y,T) = amp(x,y,T) \times NR$$

where $A(x,y,T)$ is the cumulative signal due to the glow in a sequence, $amp(x,y,T)$ is the amplifier glow signal per readout (a function of the pixel location (x,y) , the amp-on time, and the temperature), and NR is the total number of readouts of the array since the last reset. In the corners of a full, 26-readout MULTIACCUM response there will be of order 500-800 DN due to amplifier glow, as well as the associated Poisson noise from this signal. This nominal Poisson noise is propagated into the ERR array of the NICMOS calibrated images by **calnica**. Note that the temperature dependence of the amplifier glow is only corrected for when using the TEMPFIL dark reference file.

Figure 4.2: Amplifier glow images for NICMOS cameras 1, 2 and 3.

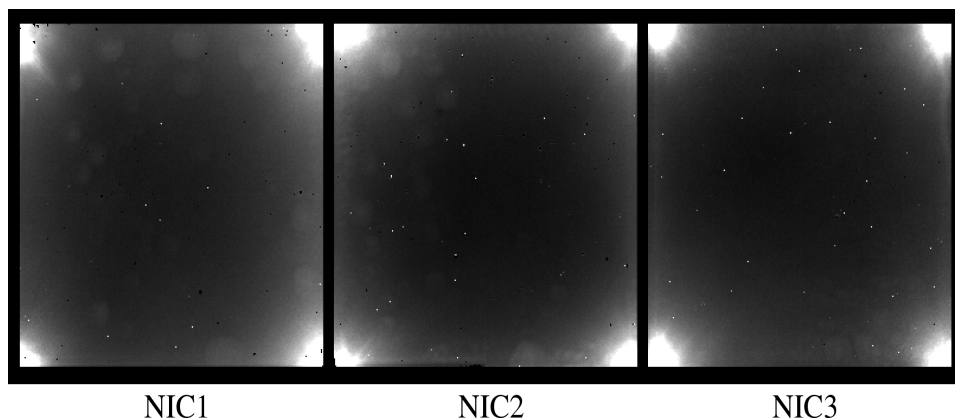

4.2.2 Bias, Shading, and “Pedestal”

There are three readily identifiable (but not necessarily physically distinct) components of the NICMOS bias: the detector reset level, shading, and variable quadrant bias or “pedestal.”

Bias Reset Level

First, a net DC bias with a large, negative value (of order -21000 ADU) is introduced when the detector is reset. This bias is different in each readout quadrant, but is essentially a constant within each quadrant, plus a fixed pattern representing the inherent pixel-to-pixel reset levels. In standard MULTIACCUM processing, this is removed by subtracting the so-called “*zeroth readout*” of the image from all subsequent readouts, e.g. in the ZOFFCORR step of *calnica*. It is therefore not a component of any calibration reference file, but is removed using the zeroth readout of the science image itself.


Shading

Shading is a noiseless signal gradient, a pixel-dependent bias, which changes in the direction of the pixel clocking during a readout. This bias change is caused by a temperature dependence of the readout amplifier bias. The amplifier temperature changes rapidly during the readout of the array. The result is a bias which changes considerably between the time the first and last pixels of a quadrant are read. Visually, this appears as a ripple and a signal gradient across a given quadrant of an uncorrected image (Figure 4.3). The amplitude of the shading can be as large as several hundred electrons across a quadrant in NIC2, with smaller amplitudes in NIC1 and NIC3. The shading exhibits all the characteristics of a bias change, including lack of noise.

The shading signal is not the same for each readout, but depends primarily on the time interval since the last readout (not reset) of a pixel. For each readout in a NICMOS MULTIACCUM sequence, this time

interval is recorded in the FITS header of each imset by the keyword DELTATIME. If the time Δt between reads remains constant, the bias level introduced by the shading remains constant, but if Δt varies (e.g. logarithmically, as in some MULTIACCUM sample sequences), then the bias level changes with each successive read, and thus the overall shading pattern evolves throughout the sequence.

Figure 4.3: Examples of shading for NICMOS cameras 1, 2 and 3

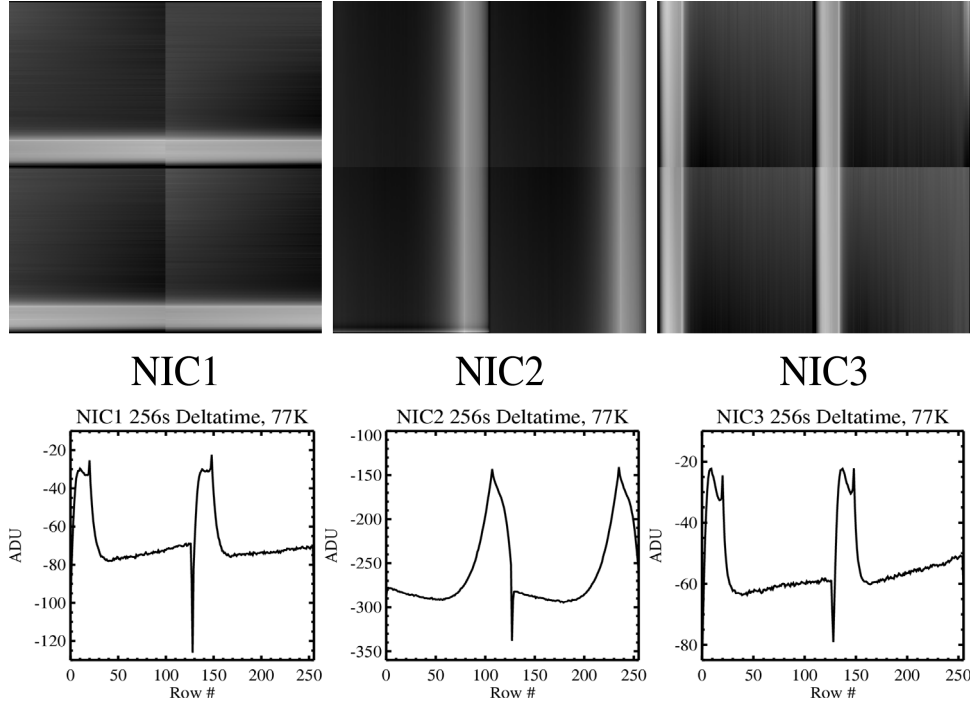

In addition to the DELTATIME dependence, the shading amplitude and shape also depend on the mean temperature of the detectors, which slowly warmed as the cryogen sublimated over Cycle 7, and has also shown to vary since the installation of the NCS. See Section 4.2.3 for a discussion on dark reference files that corrects for this temperature dependence. Subtle temperature changes during a MULTIACCUM exposure can also lead to shading changes. A sequence with many long DELTATIMES (such as a SPARS256) can cool between the first and last reads, resulting in a "DELTATIME=256s" shading that is different in the 25th read than it was in the 4th read. Numerically, shading is of the form:

$$S(x,y) = s(\Delta t, x, y, T)$$

where the shading s is a function of the pixel location, DELTATIME Δt and detector temperature T .

Variable Quadrant Bias or “Pedestal”

In addition to the net quadrant bias introduced at array reset, there is some additional offset which is time-variable and, to some degree, stochastic. This variable quadrant bias has been described as the “*pedestal effect*” in many discussions of NICMOS data, although we note here that the term “pedestal” has also been applied to other aspects of NICMOS array behavior. The variable quadrant bias is usually constant over a given array quadrant, but different from one quadrant to another. Its amplitude varies from readout to readout, sometimes drifting gradually, but occasionally with sharp changes from one readout to another (not always seen in all quadrants simultaneously).

On 22 August 1997, a modification was made to the NICMOS flight software which reduced but did not eliminate the pedestal effect. Data taken before that date is, in general, severely affected by variable bias levels, and requires careful handling in order to achieve high quality data reductions. However, essentially all NICMOS data, even after the flight software change, are impacted by pedestal to one degree or another.

The variable quadrant bias has two major effects on NICMOS MULTIACCUM data. The first (and generally less important) effect is that the signal in a given pixel, which should normally accumulate linearly with time over the course of an integration (after other sources of bias and dark current are removed, and when intrinsic array non-linearity is corrected), can instead vary irregularly as the bias level in a quadrant changes “underneath” the astronomical signal from source + background. The CRIDCALC step of the **calnica** pipeline fits a linear ramp (counts vs. time) to the accumulating signal in the MULTIACCUM to derive the source + background count rate, with a rejection procedure designed to eliminate transient cosmic ray events (see Section 3.3.2 and Section 4.9). A varying bias level can improperly trigger the CRIDCALC cosmic ray rejection or reduce its sensitivity to real cosmic ray events.

Secondly, the net bias change over the course of the exposure results in an additive offset (different in each quadrant) when the MULTIACCUM sequence is reduced to a single count rate image (the *_cal.fits file) by CRIDCALC. When the image is flat-fielded, this undesired, additive offset is then modulated by the flat-field, and appears as an inverse flat-field pattern in the final, reduced data. For illustration, consider an image where the incident astronomical flux (sources plus sky background) is given by $S(x,y)$. This is modulated by the spatially dependent quantum efficiency, or flat field, $Q(x,y)$. To this is added a quadrant bias offset B_q , which may be different in each quadrant. Here we neglect all other sources of bias and dark current, assuming that they can be adequately removed by standard processing. The recorded raw image is $I(x,y)$:


$$I(x,y) = S(x,y) \times Q(x,y) + B_q$$

If this image were then divided by the flat field (or, to follow the STScI pipeline convention, multiplied by the inverse flat field), the result would be:

$$I(x,y) * Q^{-1}(x,y) = S(x,y) + B_q \times Q^{-1}(x,y).$$

Thus, the desired image $S(x,y)$ is recovered, but an additive, inverse flat-field pattern is also present, with an amplitude that may be different for each quadrant. These inverse flat patterns, along with discontinuities between quadrants, are the typical hallmarks of a pedestal problem in processed NICMOS data (see example in Figure 4.4).

Figure 4.4: Data affected by variable quadrant bias.

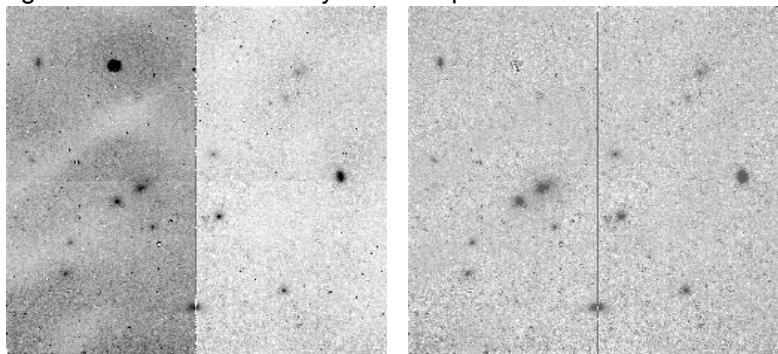

Left: image processed normally with **calnica**; note the quadrant intensity offsets, and also the residual flat-field pattern imprinted on the data, due to the unremoved bias being multiplied by the inverse flat. **Right:** image after processing through **pedsky**

It is important to note here that a residual flat-fielding pattern may also arise from reasons completely unrelated to pedestal. In particular, the NICMOS flat fields have a strong color dependence, and the spectrum of the background (especially at longer wavelengths where thermal emission dominates) does not necessarily match that of the lamps used to create the flat fields. Residual patterns may therefore sometimes result from division by standard internal lamp flats, again especially at longer wavelengths in the medium and broad band filters. We return to this point in Section 4.2.4 in the discussion of the **pedsky** software routine and again in Section 4.6.2. Unremoved shading also introduces a bias offset (but a positionally dependent one) which, when multiplied through by the inverse flat field, will create a pedestal-like effect.


The unpredictable nature of this variable quadrant bias means that it is not possible to remove it with standard reference frames. (In passing, we note that it also considerably complicates the task of generating “clean” calibration reference files of any sort in the first place.) The user must attempt to determine the bias level from the data themselves and subtract it before flat fielding the data. The difficulty, then, is determining the bias level independent of the sky + source signal present in the data. No one method has been developed which does this equally well for all types of

NICMOS data. The methods which have been tried depend on the nature of the target being observed, e.g. sparse fields consisting mostly of blank sky are treated differently from images containing large, extended objects or crowded fields. We discuss pedestal removal techniques in Section 4.2.4 below.

Bias Jumps or Bands

Occasionally, spatial bias jumps (sometimes called *bands*) are seen in NICMOS images (Figure 4.5). These are apparently caused by a bias change when the amplifiers of one NICMOS camera are being used at the same time as another is reading out. They are very commonly seen in the last readout of a MULTIACCUM sequence, but may occasionally occur in intermediate readouts as well. A flight software change was made prior to Cycle 11 to help mitigate this problem and as a result it is rarely seen in data taken after January 1, 2000 (Cycle 11 and onwards).

Figure 4.5: Bias jumps or “bands” in a NICMOS image.

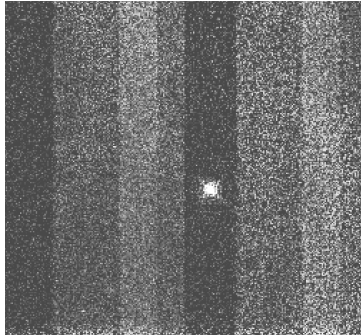

4.2.3 Dark Reference Files

Improved Temperature-Dependent Darks

A new set of temperature-dependent dark reference files have been created that incorporate all aspects of the dark current. These files consist of several extensions, each composing one component of the total dark current. Separate extensions represent the linear dark component, the amp glow, and each of 12 different DELTATIMEs shading component. The temperature-dependent, comprehensive dark current reference file names are recorded in the science header keyword `TEMPFILE`. For further updates please refer to the NICMOS Web page at:

<http://www.stsci.edu/hst/nicmos>

Calnica versions 4.2 or later use these files and is also backwards compatible with older non-temperature dependent reference files. See the **calnica** helpfile (DARKCORR section) in **STSDAS** for details. Users can recalibrate their data using **calnica** and the latest reference files by using either the **STSDAS** package in **IRAF**, or by requesting the calibrated data

products from the HST data archive. The OTFR will use the appropriate dark reference files as the data is extracted from the archive.

Historically, the mounting cup temperatures were used to represent the best known temperature of the detectors. This temperature is stored in the NDWTMP11 (for NIC1 and NIC2) and the NDWTMP13 (for NIC3) keywords in the *_spt.fits files. The use of the mounting cup temperature for determining appropriate dark components has been superseded by the use of the Bias-derived temperature. See Section 3.3.1 for details.

Random Uncertainties (i.e., noise) in the Temperature-Dependent Darks

In the center of the NICMOS arrays, where the effects of shading and amplifier glow are smallest, the uncertainties in the dark reference files are dominated by the readout noise, and to some extent the higher dark current at the NCS operating temperature. The older STScI synthetic darks were typically based on an average of about 15 measurements per readout sample per pixel. Therefore the estimated pixel-to-pixel uncertainties in the dark reference files are of the order of 1 DN (about 5 electrons). In the corners of the arrays the amplifier glow is the largest source of noise, increasing as a function of the number of readouts. For the largest number of readouts (26) the estimated uncertainty is of the order of 5 DN (about 27 electrons). It is important to note that the effect of these "random uncertainties" in the calibration files on science data is not actually "random," however. The pixel-to-pixel noise pattern in the dark reference files is systematically imprinted on all science images from which they are subtracted. This can introduce a sort of "pattern noise" in the images, which is apparently random but actually affects the pixel-to-pixel statistics of reduced data in a systematic way. In general, this is not a limiting source of noise in NICMOS data, but it can set a limit to the pixel-to-pixel noise achievable with images reduced by **calnica** using the standard reference files.

In the newer, temperature-dependent dark reference files (TEMPFILE), a much larger number of dark exposures has been averaged to produce the final product, thus reducing this pixel-to-pixel component of the dark frame "noise" to a lower level.

Systematic Uncertainties in the Temperature-Dependent Darks

The dark current pedestal adds some uncertainty to the darks, since on-orbit dark frames are used to generate the calibration reference files. In essence, the pedestal makes it difficult to establish the absolute DC level of the dark current. However, every effort was made to minimize the effects of the pedestal when making the reference files currently in the database. Persistence (charge trapping, see Section 4.7) from the amplifier glow following long periods of auto flushing when the detectors are not exposing (such as during Earth occultations) can often be seen faintly in

some exposures. This is most often seen as residual "brighter" corners in the first exposure of an orbit if that exposure is long enough to detect it. Usually by the second half of the orbit this has decayed enough that it is not seen. See Section 4.2.4 below for information on mitigating this effect.

On Orbit Darks

All dark images taken with NICMOS are available through the *HST* Archive. However, observers wishing to use on-orbit dark data obtained at conditions as similar as possible to the science data, may retrieve darks for the camera of interest with the appropriate MULTIACCUM sequence and the correct number of readouts (NSAMP), process them by subtracting the zeroth readout (ZOFFCORR), and combine them on a readout-by-readout basis with some suitable rejection scheme to eliminate cosmic rays (e.g. median or sigma clipping).

In practice there are several difficulties when doing this. First, on-orbit darks are affected by pedestal effects. Care must be taken when averaging frames, particularly with sigma rejection schemes, since the DC bias level of a given quadrant in a given readout may vary considerably from image to image. The average dark image will still have some mean pedestal value in it. Second, one should be careful to examine all dark frames used for the average, and to discard images which are adversely affected by bright object and SAA-induced persistent signal (see Section 4.8.2 below). Finally, because shading is temperature dependent, care should be taken to combine darks taken at the same detector temperature (within approximately 0.1 degrees K) as the observations for which they will be used. All of the effects described under the random and systematic uncertainties of the Temperature-dependent darks will generally apply when making dark reference files directly from observed dark observations.

ACCUM and BRIGHTOBJ Mode Darks


In principle, ACCUM mode allows the user to specify any of a large number (173, to be precise) of possible exposure times, ranging from 0.57 to 3600 seconds, and up to 25 initial and final readouts (NREAD), even though only values of 1 and 9 are supported by STScI. As was discussed above, the various components of the dark reference files (e.g., bias shading, linear dark current, and amplifier glow) depend not only on the integration time, but on the number of readouts and the readout delta time intervals. Therefore each and every combination of ACCUM exposure time and NREAD requires a unique dark image for calibration, and it was not practical to calibrate all of these on orbit. In addition, as has also been noted, the shading (particularly for NIC2) also depends on the instrument temperature.

At the present time, there are no "standard" dark calibration reference files available from the HST Calibration Database for use with ACCUM mode data. The dark reference files used for processing ACCUM mode

images in the OPUS pipeline were dummies. In principle it is possible to create ACCUM mode darks from the TEMPFILE (temperature-dependent dark) reference files using a procedure similar to that which has been used for MULTIACCUM data by interpolating the shading between the measured delta times in the standard sequences and properly scaling the amp glow. In addition, many individual on-orbit ACCUM mode dark exposures are available from the Archive, and it is not unlikely that for any given ACCUM mode science exposure there will be darks available with the right exposure time (if not necessarily the right temperature). If you need to calibrate ACCUM mode science images, you should search the Archive to see if suitable darks are available, or discuss the matter with your Contact Scientist.

In general, BRIGHTOBJ mode exposures are so short that true linear dark current is negligible. Moreover, by design they are generally used only for very bright targets, and most sources of dark and bias are relatively unimportant compared to the object signal. The BRIGHTOBJ exposures that have been taken to date show low-level alternating column or row striping (depending on camera) which subtracts well by using either a dark exposure of corresponding length or by creating a median or column/row collapse median (see Figure 4.6). A set of dark reference files have been created for the exposure time/camera combinations that have been used so far, namely 1, 2, 5, and 10 milliseconds for both NIC1 and NIC2. There are no NIC3 BRIGHTOBJ observations to date. These darks are available upon request and are installed in the calibration database. It should also be noted that BRIGHTOBJ mode is known to be highly nonlinear and a characterization of that nonlinearity is underway, but the mode should currently be considered photometrically unusable. BRIGHTOBJ exposures are however useful for acquisitions of very bright sources (e.g. for the NIC2 coronagraph), as PSF centroiding is still possible, and this has been done successfully in the past.

Figure 4.6: NIC2 0.001024 BRIGHTOBJ mode exposure of HD10700

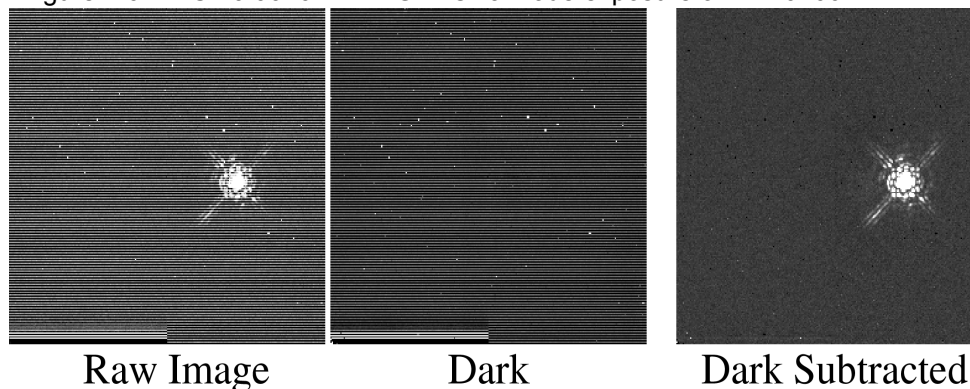

4.2.4 Cures: How To Get Rid of What's Left

Several components of the bias/dark may not be adequately removed by the standard pipeline dark correction for a variety of reasons. In particular, residual shading in NIC2 data, bias drifts and jumps, ampglow persistence and the net pedestal may still be present after standard processing. Here we describe ways of handling each of these.

Residual Dark Current and Shading

Even when using the new temperature-dependent dark reference files some shading and linear dark current residuals can be left in the calibrated data. There are a number of ways to handle temperature driven residuals in calibrated data. The shading residual is likely to be very small given the relatively stable temperature and small shading versus temperature amplitude. In most cases the delta-shading can be assumed to be a constant across the array. Any shape change will be a second order effect. The **STSDAS** task **biaseq** described in the next section is a good way to do this, essentially treating the residual shading as a “pedestal” term.

Residual dark current is more difficult to handle, as it is extremely sensitive to small temperature changes. Most of the linear dark component is due to thermal generation and recombination in the bulk HgCdTe. Each pixel can be thought of as an independent diode, and as such each will have its own personalized temperature dependence which varies exponentially with $1/T$. In addition, elevated dark current near the corners of the array is likely due to a combination of charge trapped amp-glow signal (ampglow persistence) and localized thermal heating by the output amplifiers. Because of this it is usually not possible to linearly scale and subtract an image of the dark current to minimize residuals. A scale factor that corrects one pixel will be incorrect to apply to a neighboring pixel. It may be possible to model the dark current per-pixel, but limitations in the instantaneous temperature determination and unknown prior readout history make this difficult at present.

A number of alternate techniques have proven useful. For example if a dataset has a large number of dithers and few sources, or has a set of dithered “sky” images that were taken contemporaneously with the science data, a source-masked median sky image can be constructed from the calibrated data itself. This sky image will then contain both a map of the sky background and the median residual dark current for that set of observations. Beware though that the timescale over which the dark current is changing may be shorter than that over which the data was taken. Also if the number of images available for making such a sky image is small it may be noise limited and its application might actually degrade image quality rather than improve it. The same is true of darks taken as a part of a science program, and in that case the darks must have been taken some time before or after the observations themselves. As always with sky images

constructed from science data, care must be taken not to subtract data from itself.

Some success has been achieved by trying to match darks to observations based on previous observational history. For example, if a program is taking two long exposures per orbit, it may be possible to find a set of dark (or sky) images that were taken in an identical manner and construct two separate darks (or skys) - one for the first half of the orbit and one for the second half. This at least gives a correction over two time domains instead of averaging over the entire orbit. This tends to work well at removing the large spatial scale dark current residuals, but the warmest pixels are still poorly corrected because of their higher temperature sensitivity. Only programs with certain observational constraints can take advantage of this.

Another option for dealing with the “salty” and most temperature sensitive high-count-rate pixels is to simply treat them as bad pixels. If the science data was dithered, these pixels can be masked before combination (when averaging or drizzling) and be rejected just as cosmic ray hits would be. The large number of such pixels (see Figure 4.1) may make this impractical for programs that are sparsely dithered.

Variable Quadrant Bias or “Pedestal”

Variable quadrant bias or “pedestal” is not removed by standard processing. STScI has distributed several **STSDAS** tools for removing this variable bias level. Here we briefly describe the tools that are currently available in the **stsdas.hst_calib.nicmos** package.

biaseq

The **biaseq** task in the **stsdas.hst_calib.nicmos** package is designed to remove the changes in quadrant bias level from readout to readout during the course of a MULTIACCUM exposure. It adjusts the bias levels in each NICMOS quadrant so that the net counts in that quadrant increase linearly with time. This “bias equalization” procedure does *not* remove the net bias offset that produces the pedestal effect. Essentially, it removes any temporally non-linear components of the bias drift, i.e., the second and higher order time derivatives of the bias, but leaves an unknown linear term in the bias drift (i.e., the first time derivative). The program cannot distinguish between this linear bias drift and an actual, linearly accumulating astronomical signal, and thus leaves the linear bias term in the data so that it must be removed by some other method (see “pedsky” and “pedsub” below). In principle, **biaseq** will work on any NICMOS MULTIACCUM image, regardless of the nature of the astronomical sources present, provided that there are enough MULTIACCUM samples available. As a by-product, **biaseq** can also attempt to identify and remove bias jumps or bands (see Section 4.2.2 above) from individual readouts.

The **biaseq** task must be run on an intermediate image file (*_ima.fits) which is produced by partially processing a raw NICMOS

data set through only the first few processing steps of **calnica**. The pipeline processing steps **BIASCORR**, **ZOFFCORR**, **ZSIGCORR**, **MASKCORR**, **NOISCALC**, **NLINCORR**, **DARKCORR** and **BARSCORR** should be performed before running **biaseq**, but not **FLATCORR**, **UNITCORR** or **CRIDCALC**, i.e., the image should not be flat fielded and should be in units of counts (not counts per second). The **nicpipe** task in the **stdas.hst_calib.nicmos** package provides a convenient way to carry out the partial **calnica** processing needed as preparation for **biaseq** (see example below, and also Section 5.1).

The **biaseq** task assumes that the astronomical signal (sky plus sources) accumulates linearly with time, and that any non-linear behavior is due to changing bias levels that are constant within each array quadrant, except perhaps for bias jumps. If these assumptions are not correct, then the task may not work properly. For example, if the sky background is changing with time, either because it is dominated by variable thermal emission or because of scattered earthlight (see Section 4.10), then the routine may not function correctly. The **nicmos** task **pstats** may be used to compute and graph data statistics versus time or readout number, which can help to identify time-varying background levels. Objects which saturate the NICMOS array will also no longer accumulate signal linearly with time. However, in this case, unless a large fraction of the pixels in a quadrant are saturated, there should be no noticeable effect on **biaseq**. Also, residual shading may result in a bias which changes from readout to readout but is not constant across the quadrant, and this may also cause problems for **biaseq**. In particular, residual shading can improperly trigger the bias jump finding algorithm. If there is residual shading in the images, it should be removed with a temperature-dependent shading correction (see “Residual Dark Current and Shading” on page 85) before running **biaseq**. If **biaseq** is run without doing this, the user should at least disable the bias jump finding option. The **biaseq** help pages give further information about this task and its parameters.

pedsky

For NICMOS images of relatively blank fields, free of very bright or large sources which fill a substantial portion of the field of view, the **pedsky** task may be used to measure and remove an estimate of the sky background and quadrant-dependent residual bias (or “pedestal”). The task depends on having a large fraction of the image filled by “blank” sky, and thus may not work well for images of large, extended objects or very crowded fields.

Pedsky runs on a single science image (i.e. not on all the separate readouts of a NICMOS MULTIACCUM file). It operates only on the `[SCI,1]` extension, which is appropriate when the task is run on, e.g., the `*_cal.fits` images that are the final product of the **calnica** calibration pipeline. The task’s internal algorithms operate on an unflat-fielded image, but a fully-calibrated (including flat fielding) image may be used as input,

as the task will check the status of the flat fielding (via the value of the FLATDONE keyword in the input image header) and will temporarily remove and, at the end of processing, reapply the flat field if necessary. Note, however, that the FLATFILE used for the processing *must* be available locally in order to run `pedsky`. Therefore if you wish to use this task on reduced data taken from the *HST* Archive, be sure to retrieve the appropriate flat-field reference file as well.

Following the discussion in Section 4.2.2 above, let us say that a NICMOS image $I(x,y)$ may be described as

$$I(x,y) = S(x,y) \times Q(x,y) + B_q$$

where $S(x,y)$ is the incident astronomical flux (sources plus sky background), $Q(x,y)$ is the flat field, and B_q is the quadrant-dependent bias offset. The **pedsky** task works by minimizing the quantity

$$X^2 = \sum_{xy} (I_{xy} - S \times Q_{xy} - B_q)^2$$

which is a measure of the total image variance, as a function of the sky level S and four quadrant bias levels B_q . Here we have made the simplifying assumption that the “true” incident flux $S(x,y)$ in a relatively blank-field image can be approximated as a constant sky background S , i.e. that there are no sources present. In real data where there are real sources, the quantity X^2 includes a contribution due to the presence of actual objects in the image, above the assumed uniform, constant sky level S . The impact of these sources is minimized, however, by using sigma-clipped statistics which exclude pixels with strongly deviant values, e.g. those due to actual astronomical sources, bad pixels, etc. Additionally, the user may apply a ring median filter to the image when computing X^2 . This can effectively remove compact or point-like sources, and may help the task perform better for moderately crowded fields, but considerably slows the computation speed. The user may wish to experiment by trying **pedsky** both with and without the ring median option. In practice, a certain amount of “source noise” contribution to X^2 is tolerable to the **pedsky** algorithm. It acts as an offset to the amplitude of X^2 , but generally has no effect on the location of the minimum value for X^2 relative to S or B_q .

Pedsky works in both interactive and non interactive modes. Alternatively, the user can supply a sky value to be subtracted, in which case the remaining quadrant-dependent pedestal is estimated and subtracted. After **pedsky** processing, the remaining standard calibration steps, including flat fielding, can then be easily applied using another call to the script **nicpipe**.

Note that, in principle, any image may be used to represent the spatial structure of the sky, i.e., you do not need to use a standard NICMOS flat-field reference file. In particular, for some NICMOS images the two-dimensional structure of the sky may not exactly resemble that of the flat field. This may happen for at least two reasons. First, as will be

discussed below (Section 4.6.3), the NICMOS flat fields are strongly color dependent, and the spectrum of the internal flat-field lamps does not necessarily match that of the sky background, especially at longer wavelengths ($> 1.8 \mu\text{m}$) where thermal emission begins to dominate over the zodiacal sky. The result is that the spatial structure of the sky may not be quite the same as that of the flat field, and that the sky multiplied by the inverse flat reference file may have some residual structure which correlates with the flat-field pattern and contributes to the total image variance X^2 measured by **pedsky**. This can confuse **pedsky**, resulting in improper sky and pedestal measurement. This problem is most important for images dominated by thermal background, but may also affect shorter wavelength data, especially for NIC3 data where the ratio of background counts to quadrant bias offset amplitude is larger than for the other two cameras. Second, at longer wavelengths, the thermal background generated within the telescope may illuminate the detector differently than does the zodiacal sky, and thus the overall background may not match the QE response pattern measured in the flat field.

In cases like these, you may want to provide your own “sky” images for use by **pedsky**, rather than rely on the flat-field reference files to represent the shape of the sky. One possibility would be to use sky frames constructed from the median of many dithered science or background exposures. This can sometimes improve the quality of the sky + pedestal fitting even for data taken at shorter wavelengths. This was the approach taken for STScI reductions of the HDF-South NICMOS data, for example. Another possibility, especially for long wavelength data, might be to use a specially-constructed color-dependent flat field (see Section 4.6.3). The **pedsky** help pages give further information about this task and its parameters, including guidance for how to use images other than the flat field as the sky model.

pedsub

As described above, the **pedsky** task requires lots of “blank” sky to be effective, and will only work on relatively sparse NICMOS images. The **pedsub** task provides an alternative method for images which contain larger objects that fill the field of view. The basic methodology for **pedsub** is essentially the same as that of **pedsky**, modeling the image as the sum of a constant (per quadrant) pedestal offset plus an astronomical signal (sky + objects) that is modulated by the flat field, and then loops over a range of trial values for the pedestal signal, searching for the amplitude which minimizes pixel-to-pixel variations. Unlike **pedsky**, however, **pedsub** can optionally apply a spatial filtering function to each trial image in order to remove unwanted features or spatial frequencies (i.e., the signal from objects) that might bias the calculation of the pixel value spread. The filtering options are “median” and “mask,” which essentially carry out low-pass and high-pass filtering of spatial frequencies. The “mask” option removes all large-scale structure from the trial image, leaving the RMS

minimization process to operate only on the small-scale, pixel-to-pixel component of the flat-field signal. This option can be effective when trying to measure and remove pedestal from, e.g., images of large galaxies.

Pedsub has many other parameters and options which are fully described in the **STSDAS** help pages for the task. These should be consulted carefully before using the task, and the user may wish to experiment with combinations of these parameters in order to achieve the best results.

Using **nicpipe**, **biaseq** and **pedsky**: An Example.

Here we illustrate the use of the **nicpipe**, **biaseq** and **pedsky** tasks with one example. A similar sequence could be used with **pedsub** substituted for **pedsky**. The raw data frame is `n4ux23x0q_raw.fits`. This is a NIC3 image taken with the SPARS64 readout sequence and NSAMP=25. We might start by using the **sampinfo** task (see Section 5.1) to look at the details of the readout sequence.

```
ni> sampinfo n4ux23x0q_raw.fits
```

This will produce a table of output information that looks like this:

IMAGE	NEXTEND	SAMP_SEQ	NSAMP	EXPTIME
n4ux23x0q_raw.fits	125	SPARS64	25	1407.933
IMSET	SAMPNUM	SAMPTIME	DELTATIME	
1	24	1407.933	63.997	
2	23	1343.936	63.997	
3	22	1279.939	63.997	
...	
21	4	127.990	63.997	
22	3	63.993	63.388	
23	2	0.605	0.302	
24	1	0.302	0.302	
25	0	0.000	0.000	

We see that the readouts with linearly spaced DELTATIME values (SAMPNUMs 4 through 24) are in imsets 1 to 21. The last readout (imset 1) often has bias jumps (see “Bias Jumps or Bands” on page 81), so we may want to exclude it when feeding the desired range of sky samples to **biaseq** for use in constructing the “clean” sky image. So:

```
ni> nicpipe n4ux23x0q_raw.fits "" stage=biaseq
ni> biaseq n4ux23x0q_ima.fits n4ux23x0q_beq.fits \
>>> skysamps=2-21 fitbias+ fitjump+
```

The output image `n4ux23x0q_beq.fits` has been corrected for non-linear bias drifts and for spatial bias jumps as well.

Next, we complete the pipeline processing using **nicpipe**, doing the FLATCORR, UNITCORR, CRIDCALC steps to prepare for **pedsky**:

```
ni> nicpipe n4ux23x0q_beq.fits "" stage=final
```

We now run **pedsky** non-interactively, letting it fit for the sky level and four quadrant biases on its own.

```
ni> pedsky n4ux23x0q_beq_ima.fits n4ux23x0q_ped.fits \
>>> salgorithm=auto interactive- rmedian-
```

The end product, `n4ux23x0q_ped.fits`, is the fully processed and pedestal corrected image.

Other Pedestal Removal Software

In addition, there are other, “freelance” packages for NICMOS data reduction. One example is Brian McLeod’s **NICRED** package (McLeod 1997, in the proceedings for the 1997 *HST* Calibration Workshop, ed. S. Casertano et al., p. 281), which offers a general suite of NICMOS data reduction tools, including routines which estimate and subtract pedestal. Ultimately, there are similarities in the pedestal removal methods used by **pedsky**, **pedsub**, and the **NICRED** algorithms, and therefore it should be possible, in principle, to unify them in a single task.

4.3 Bars

Bars (Figure 4.7) are another bias-related artifact mainly affecting Cycle 7 and 7N data, which have now been mitigated by the BARSCORR step in calnica. Data from Cycle 11 and beyond are not likely to be affected. Bars appear as narrow stripes that cross the quadrants of an array, and occur identically in all 4 quadrants at the same rows/columns in each. They arise from electrical cross-talk in the detector lines when one camera reads out while the auto-flush pattern is executing in one or both parallel cameras. If an observation was made with all three cameras running in parallel using the same readout sequences, then there usually are no bars present in the data because there is no collision between camera readouts and parallel detector autoflush.

The bars run along the slow readout direction, i.e. along columns in NIC1, and along rows in NIC2 and NIC3. Normally there is only one bar per quadrant, but occasionally there are more, always reflected in all 4 quadrants. Sometimes the bars will be in sync, appearing at the same place

in successive readouts. Other times, they may appear in alternate readouts, or their positions may vary from readout to readout, sometimes appearing to march across the frame over the course of a MULTIACCUM sequence. They typically run the length of a quadrant (128 pixels), and are 3 pixels wide. The first pixel is lower than the mean, the second is at the mean level and the third is higher than the mean, giving the impression of an undersampled sinusoidal spike with an amplitude of up to ~ 10 DN peak-to-peak. The bars are almost always broken in at least one place, with a shift of 2-10 pixels in the narrow direction.


A flight software change was made prior to Cycle 11 to help mitigate this problem by automatically turning off the autoflush sequence in unused parallel cameras. If no NICMOS parallel cameras were being used at the time of an observation, then there will be no bars in data taken after 1/1/2000 (Cycle 11 onwards). If a parallel camera is used with the same readout sequence, then as before, no bars will be present. However if a parallel camera is used with a different readout sequence then it still can induce bars in the other camera readouts, even in data taken after 1/1/2000. The software change has dramatically decreased the incidence of the bars in prime-only exposures and they are rarely seen now.

Cures:

The bars are noiseless, localized changes in detector bias. The amplitude is usually quite low, and for some observers they may have little impact on science data. However, it is possible to correct bars during post-processing of data obtained prior to Cycle 11, or newer data still affected by the electronic band problems. One approach is to flag pixels affected by bars in the data quality (DQ) array for each imset where the bars occur, e.g., by setting the DQ values to the bad data flag value 256. Subsequently, when **calnica** carries out the CRIDCALC step, fitting the counts versus time to determine the count rates, it will ignore flagged pixels in a given imset, and the bars will therefore not perturb the fits. A memo describing this procedure is available as a link from the STScI NICMOS Data Anomalies Web page.

If a bar appears in the zeroth readout, it will be subtracted from all the other readouts as part of the normal calibration process (ZOFFCORR), and appear as a negative bar pattern in all readouts of the processed `*_ima.fits` file. This should have no significant effect on the calibrated final image (`*_cal.fits`), however, since the bar just acts as an intercept offset to fit of counts versus time, which is irrelevant to CRIDCALC which only computes the slope (i.e. the count rate).

Figure 4.7: Bars in a NICMOS Camera 1 Image.

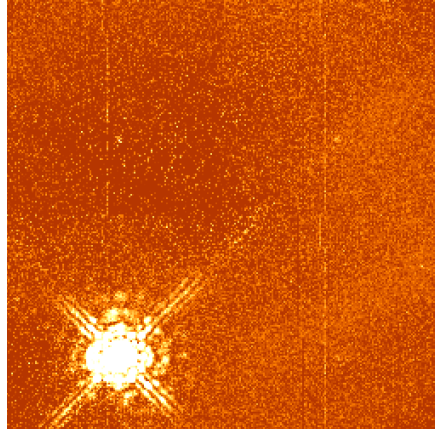

4.4 Detector Nonlinearity Issues

4.4.1 Nonlinearity Calibrations

The response of the NICMOS detectors is inherently nonlinear. As was described in Section 3.3.2, the **calnica** pipeline applies a nonlinearity correction with the step NLINCORR. Early nonlinearity calibrations, used for all Cycle 7 and 7N data processed retrieved from the *HST* Archive before 26 September 2001, used a low-order correction, which worked well for most purposes. However, the STScI NICMOS group has subsequently re-calibrated the detector nonlinearities and produced improved NLINFILE reference files. There are two significant changes:

- In the old nonlinearity calibrations, data values below a minimum threshold (set for each pixel by the value in the [NODE, 1] extension of the nonlinearity reference file) had no calibration applied. However, NICMOS data are actually nonlinear at all levels, and in the new reference files the linearity correction will be calibrated and applied at all count levels.
- Previously, only corrections of the form $F_c = (c_1 + c_2 * F) * F$ were allowed. The new reference files and software will permit 2nd order corrections terms which improve the accuracy of the linearity calibration (see Section 3.3.2).

The new nonlinearity reference files are now used by default when data are retrieved from the archive and processed by OTFR. Version 3.3 and later versions of **calnica** accommodate second order correction scheme used in the new reference files.

4.4.2 Non-Zero zeroth Read Correction for Bright Sources

As described in Section 4.2.2 above, the first non-destructive readout after a reset provides the reference bias level for the counts in each pixel of a NICMOS science image. This “zeroth readout” is transmitted to the ground with MULTIACCUM data, but is directly subtracted from the final readouts on-board the telescope for all the other readout modes. Due to physical limitation in the readout speed, the zeroth read happens 0.203 seconds after the reset of the detector. NICMOS does not have a shutter, and therefore when a bright source is being observed, a non-negligible amount of charge may accumulate on the detector by the time the zeroth read is performed, enough to significantly affect detector nonlinearity. However, zeroth read subtraction is the first step of the calibration processing for MULTIACCUM data (ZOFFCORR in **calnica**), and is automatically done on-board the telescope from the final read in a ACCUM exposure. The zeroth read signal information is therefore lost before nonlinearity correction (NLINCORR in **calnica**) is performed, and for bright sources this correction may therefore be inaccurate.

Cures:

In November 1997, an additional step was added to the **calnica** pipeline processing software (version 3.0 and higher) to account for this zero read signal correction, and an additional keyword, ZSIGCORR, was included in NICMOS image headers to control this step. The ZSIGCORR step computes an estimate of the number of counts for each pixel in the zeroth readout of a MULTIACCUM, based on the count rate measured later in the exposure. This information is then used in the NLINCORR step to estimate the absolute charge in each pixel and the appropriate linearity correction for that charge level. The optional **calnica** parameter `zsthresh` controls a threshold above which the ZSIGCORR correction is made.



*If you have observed very bright targets, you should read the **calnica** documentation concerning ZSIGCORR.*

Pipeline-processed data that were retrieved from the STScI Archive before November 1997 has no ZSIGCORR correction. When reprocessing such data, the current version of **calnica** will automatically apply this step to all MULTIACCUM mode observations if both ZOFFCORR and NLINCORR are also being performed.

4.4.3 Uncorrected Saturation

Occasionally, for reasons which are not fully understood, NICMOS MULTIACCUM images of bright targets will saturate at an ADU level which is below the nominal saturation threshold specified in the nonlinearity calibration reference file. This could happen, for example, when the variable quadrant bias levels (pedestal) are at unusually large values. When this happens, the accumulating counts vs. time for the affected pixels level out at the saturated value. However, because the saturation flag is not set at the NLINCORR stage of **calnica**, when the CRIDCALC step fits “up the ramp” of counts vs. time to determine the count rate slope, it does not know to exclude the saturated data values, and fits a linear slope to a highly nonlinear data set. Among other unpleasant consequences, this tends to trigger the CRIDCALC cosmic ray detection flags, causing wholesale rejection of many or most time steps for the affected pixel. Images which have been affected by this problem will generally have anomalously low count rates for bright pixels, but the saturation flag (64) will not be set in the DQ arrays.

Cures:

The simplest cure is to modify the nonlinearity reference file to reduce the threshold where saturation flagging is triggered, and then to reprocess the data. The saturation level for each pixel is set in the [NODE,2] extension of the nonlinearity reference file. As an example, let us say that the science image is called `n4ux22hbq_raw.fits` and the corresponding nonlinearity reference file is `h7n1654cn_lin.fits`. We reduce the saturation threshold by 5%, edit the science image primary header to point to the new reference file, and reprocess:


```
ni> copy h7n1654cn_lin.fits new_nonlin.fits
ni> imarith new_nonlin.fits[NODE,2] * 0.95 \
>>> new_nonlin.fits[NODE,2] [overwrite+]
ni> hedit n4ux22hbq_raw.fits[0] NLINFILE new_nonlin.fits \
>>> update+ verify- show+
ni> calnica n4ux22hbq ""
```

If the problem reoccurs, reduce the [NODE,2] values further until the saturation threshold is properly triggered.

4.5 Count Rate Non-Linearity

The NICMOS STScI team has determined that NICMOS has a significant count rate dependent nonlinearity that also depends on wavelength. This is a different nonlinearity from the well-known total count dependent nonlinearity described in Section 4.4. The nonlinearity in amounts to 0.05-0.10 mag offset per dex change in incident flux for the shortest wavelength (F090M and F110W), about 0.03 mag/dex at F160W and less than that at longer wavelengths (see figure below). Details about how the nonlinearity was quantified can be found in the NICMOS [ISR 2006-001](#) and NICMOS [ISR 2006-002](#) Instrument Science Reports (ISRs).

Figure 4.8: Figure 4.8: Graph of non-linearity by camera, top line NIC1, middle line NIC2, and bottom line NIC3

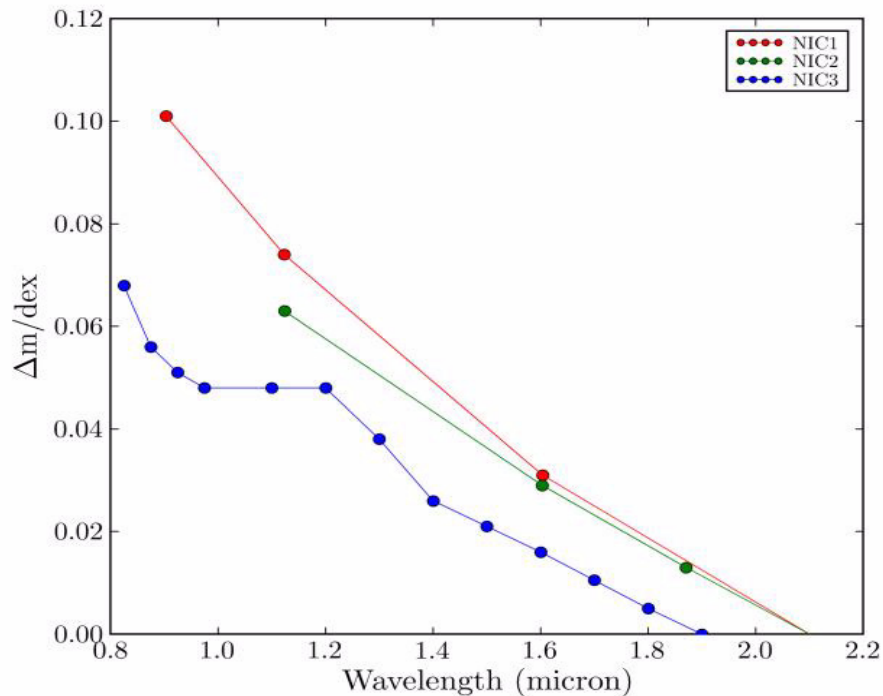

Cures:

A python routine to correct NICMOS data for the nonlinearity has been developed. The routine **rnlincor** is available in **STSDAS** as part of the NICMOS package and can be used as an independent program outside **STSDAS** as well. The routine corrects NICMOS count-rate images assuming the nonlinearity follows a power-law behavior. The wavelength dependence of the nonlinearity is interpolated between the measured points of de Jong et al. (2006, [NICMOS ISR 2006-001](#)) and Bohlin et al. (2006, [NICMOS ISR 2006-002](#)) if necessary.

While the exact cause of the count rate nonlinearity is not known, it is believed that it depends on the incoming flux only. Therefore the routine should be run on images that have been processed through the pipeline as much as possible with all instrumental effects removed. Most notably, the quadrant bias should be removed with **pedsky** or **pedsub** before performing the count rate nonlinearity correction. The **pedsky** routine subtracts the sky value, but the nonlinearity script detects this and will add that value back in (as it is part of the flux that determines the nonlinearity) before doing the correction. The routine can be run on MULTIDRIZZLED images, but this is only correct if the sky value did not vary a lot relative to the sources of interest and by making sure a typical sky value is set in the final MULTIDRIZZLED image. The routine can only be used on imaging data (pixels in grism observations receive flux from a broad range of wavelengths) and should not be applied to calibration reference files (e.g., dark frames, flat fields, etc.).

The **rnlinco** routine requires calibration tables specifying the wavelength dependence of the non-linearity and an offset to make sure the photometric zero point matches the NICMOS calibration values in the header. The filenames of these calibration tables need to be specified in the header of the images to be corrected (keywords are ZPRATTAB and RNLCOBTB). Images retrieved from the archive before this new routine was introduced will not have these header items. These header items can be added with the **IRAF** routine **hedit** or, alternatively, one can retrieve the images again from the archive.

The usage of the routine is very straightforward as it has no free parameters to influence its result:

```
> rnlinco.py infile [outfile]
```

If no output file is specified it will be created with a `_ncl` extension based on the input file name.

Little is known about the temporal variation of this effect, but the NICMOS team has a monitoring program in place. Please check for the latest information on the rate nonlinearity at:

<http://www.stsci.edu/hst/nicmos/performance/anomalies/nonlinearity.html>


4.6 Flat Fielding

4.6.1 Characteristics of NICMOS Flat Fields

NICMOS flat fields show response variation on both large and small scales. Figure 4.9 compares some of the flat field exposures used for Cycle 11 (post-NCS) calibration to those used in Cycle 7/7N (pre-NCS). It is evident that the morphology and amplitude of the variations of all three cameras is reduced in Cycle 11. This behavior is due to the fact that “cold” pixels (i.e. pixels with a lower than average responsivity) show a higher than average Detector Quantum Efficiency (DQE) increase with temperature. The flat-field variations are due also to a strong function of wavelength. At $0.8\ \mu\text{m}$, there is variation by a factor of ~ 5 (minimum to maximum) in the relative response across the array. This declines to a factor of ~ 3 at a wavelength of $2.2\ \mu\text{m}$, and at $2.5\ \mu\text{m}$ the array is almost flat. Naturally, both the spatial distribution and amplitudes of these variations are different for each camera. NIC3 has a large contiguous region with low sensitivity.

An inevitable consequence of these large DQE variations is that science data will have large spatial variations in their pixel-to-pixel noise level, and hence in signal-to-noise for sources. For images where statistics are limited by photon shot noise (either from the sources themselves or from the sky background) the S/N variations scale as the square root of the flat field amplitude (e.g., a factor of ~ 2 at F160W). Many NICMOS observations, however, especially with NIC1 and NIC2, are largely readout noise limited and for these the signal-to-noise modulation will scale linearly with the flat field, e.g., a factor of ~ 4 at F160W.

Figure 4.9: Flat-field responses for NIC1, NIC2 and NIC3.

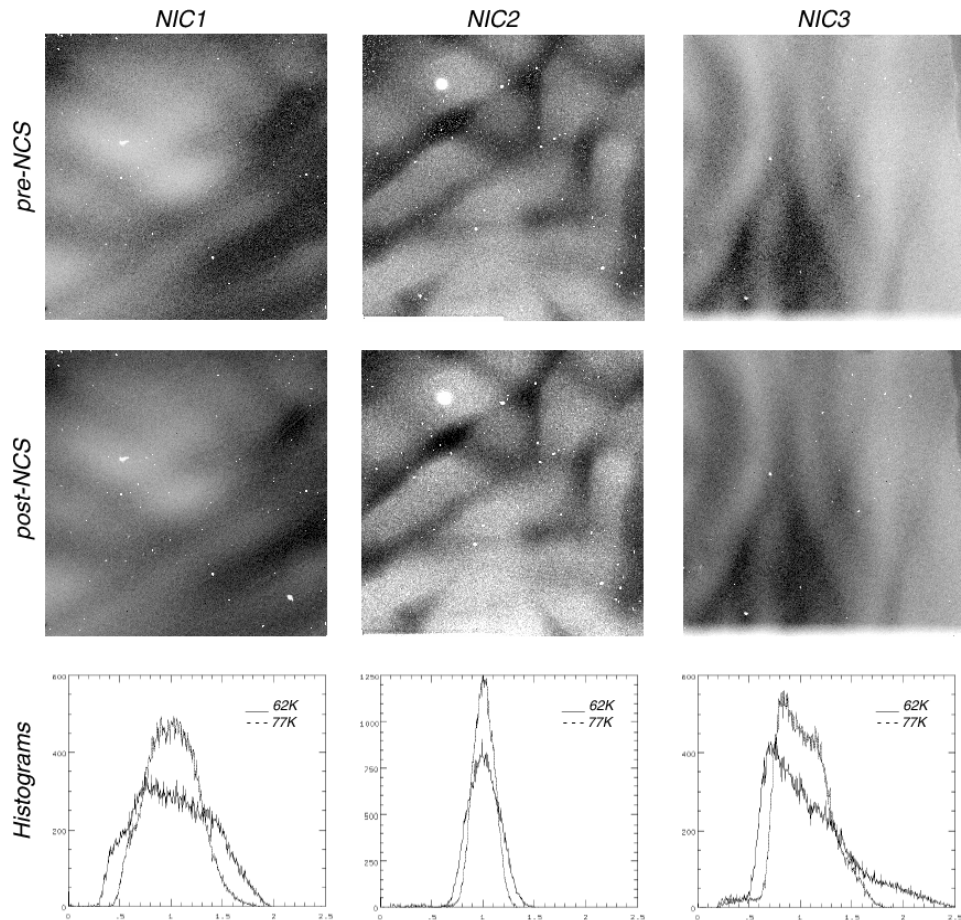

Normalized pre- and post-NCS flat-field responses for NIC1 (left) through NIC3 (right) for F110W, F187W, and F113N, respectively. The images are inverted to better display the grot; therefore the dark regions have higher QE. The color stretch is the same for both temperatures in each camera. The histograms show the “flattening” of the arrays at the higher temperature (narrower distribution). The decrease in the dynamic range between bright and faint targets is a direct result of the decreased well depth at the higher temperature.

4.6.2 Temperature-dependent Flat Fields

As with the dark current and bias, the quantum efficiency of a NICMOS detector is a function of the detector temperature. Because the instrument temperature varied somewhat throughout Cycle 7 and 7N (when operating temperature was $\sim 62\text{K}$) as well as in Cycle 11 and beyond (operating temperature $\sim 77\text{K}$), the flat-field structure also varied slightly due to this effect. For the temperature range experienced, about $\Delta T \sim 2\text{K}$ at the most, this has a relatively small effect, but does affect both the overall DQE as well as the relative structure of the flat-fields (after these have been normalized to unity). Calnica now (version 4.4 and later) uses a

temperature dependent correction factor to account for the overall DQE change (described in the PHOTCALC section in Section 3.3.2). The effect of this correction is up to a few percent depending on the detector temperature at the time of the observation. To correct also for the temperature dependent changes in the structure of the flat-fields, calnica now uses a set of temperature dependent flat-fields (version 4.4 and later). The effect of this on the photometry is at most $\sim 1\%$ and depends on the position on the detectors. Users that are concerned about their photometry at these levels and use data retrieved earlier than 2008 should consider re-calibration using the latest reference files and calnica version 4.4 (or later), or retrieve the data again from the Archive using the OTFR (see PHOTCALC and FLATCOR sections in Section 3.3.2 for more info and detailed dates). For further updates please refer to the NICMOS Web page at:

<http://www.stsci.edu/hst/nicmos>

4.6.3 Color Dependence of Flat Fields

The strong wavelength dependence of the NICMOS response may affect the quality of flat fielding for objects with extreme colors. The color of the internal flat-field lamps may not match that of the sky background, or indeed of many astronomical sources. In most cases this should only affect photometry by a few percent, but concerned users may wish to experiment with constructing customized, spectrally weighted flat fields. These can be constructed from linear combinations of (and interpolations between) existing NICMOS narrow band flat fields, as described in Storrs, Bergeron and Holfeltz 1999 (NICMOS [ISR 99-002](#)).

One situation where the color dependence of the flat fields may have a visibly noticeable effect is on the flat fielding of the sky background. The background has a significantly different spectrum than the flat-field lamps, particularly at $\lambda > 1.8\mu\text{m}$, where thermal emission from the telescope and instrument become important. After dividing by ordinary internal lamp flats, flat-field residuals may still be present in the sky background. Unfortunately, in practice it is difficult to separate these from the characteristic variations induced by the pedestal effect discussed above in Section 4.2.2. Pedestal removal routines like **pedsky** (see Section 4.2.4) key off these residual flat-field variations, and depend on having an accurate model of the spatial structure of the sky. If actual, observed sky frames are not available, then synthetic color-dependent flats may be useful when running routines like **pedsky**.

Cures:

A discussion of flat field color dependence is presented in Storrs, Bergeron and Holfeltz 1999 (NICMOS [ISR 99-002](#)). That paper describes methods for constructing color-dependent flat-field reference files, and provides **IRAF** scripts for doing so (currently applicable to Cycle 7 and 7N data, but see the NICMOS Web page for updates on this script).

In general when using NICMOS data, you should keep in mind the large spatial variations in sensitivity and signal to noise that result from the flat field structure. This can have important consequences when you are analyzing NICMOS data, requiring, e.g., careful handling when setting source detection thresholds in automatic routines like **DAOPHOT** or **SExtractor**, or for error analysis on photometry.

4.7 Pixel Defects and Bad Imaging Regions

4.7.1 Hot Pixels, Cold Pixels, and Grot

Each NICMOS array has a small number of bad pixels which may be either *cold* (i.e., very low or zero response) or *hot* (i.e., with very high or erratic dark current). Static bad pixel masks are used to set error flags (DQ=32) for these pixels in the DQ arrays during the MASKCORR step in **calnica** processing. The statistics on the cold/hot pixels present in each of the NICMOS camera are presented in Table 4.1. The cold pixels contain pixels that do not respond to incoming photons (“dead pixels”), and the hot pixels are those with increased dark current. Pixels with low responsivity or affected by “grot” (see below) are listed separately. These pixels get a flag value=16 in the MASKCORR step.

In addition to the bad pixels which were already known from ground-based testing, more pixels have shown low measured quantum efficiency in orbit. These are known as *grot* and they appear as small areas of reduced sensitivity, most likely due to flecks of anti-reflective paint which were scraped off the optical baffles between the dewars as they were forced against each other by the solid nitrogen cryogen expansion. The largest example, known as the *battleship*, is found in camera 1 and affects approximately 35 pixels. However, most grot seems to affect single pixels. Scrape tests conducted at Ball Aerospace shortly after NICMOS was launched reveal that the paint flecks can range in size from 25 μ m to greater than 100 μ m. Since NICMOS pixels are 40 μ m on a side, this means that there is potential for grot smaller than 1 pixel.

There was some concern that the warm-up and subsequent cool-down of NICMOS with the associated mechanical motions could produce an increased number of these particles. However, apart from one additional

chunk of grot in the lower right corner of camera 1, no new contaminants were apparent in the data obtained during SMOV3b in 2002. The number of pixels with significantly degraded responsivity is roughly the same now as during Cycle 7.

Table 4.1: NICMOS Cosmetics (Cycle 11 and beyond, for masks produced in March 2009)

Type	NIC 1	NIC 2	NIC 3
Cold/Hot Pixels	280	696	488
Grot	163	119	96

Cures:

Dithering is the best way to guard against the effects of bad pixels and grot. If you have multiple dither positions, you can use the static masks to exclude bad pixels when combining the images (e.g., with **calnicb**, **imcombine**, or **MultiDrizzle** with the **STSDAS dither.drizzle** routines). Or, you may interpolate over masked pixels using, e.g., **IRAF fixpix**. For further description of the mask files, see (NICMOS [ISR 99-008](#)). For further updates please refer to the NICMOS Web page at:

<http://www.stsci.edu/hst/nicmos>

Not all pixels affected by grot are unrecoverably ruined. For pixels which are only partially obscured, the effects of grot may flat field out. You may wish to compare your flat-fielded images with the grot flagged pixels to see which pixels have flattened well and which are potentially suspect.

Note that Cycle 7/7N data that were retrieved prior to April 2009 do not have the grot pixels flagged in the reference file given by the MASKFILE keyword. For these data, grot masks can be retrieved from the NICMOS Web page:

http://www.stsci.edu/hst/nicmos/calibration/reffiles/grot_mask_list.html.

Alternatively, the latest mask reference files can be retrieved from the cdb or NICMOS Web page, followed by an update of the MASKFILE keyword in the primary header of your data to point to these new reference files. Finally, you can retrieve your data again using the OTFR to ensure that all the latest update are included in your data.

4.7.2 Erratic Middle Column/Row.

In each NICMOS camera, there is one row or column which often deviates from others nearby. In NIC1 this is row 128; in NIC2 it is column 128, and in NIC3 it is column 129. Adjacent rows (or columns) are sometimes affected to a lesser degree. It is believed that this “photometrically challenged column” may be related to uncertainties in detector shading corrections. The affected column/row contains the first pixels read out in each quadrant. Since the shading function is very steep and highly nonlinear during this part of the readout, it is the part of the array most sensitive to changes in the detector environment. Thus it is thought that the pixels in these rows or columns are not any less sensitive, but that they have just had an incorrect bias subtracted from them. The result is a row or column of pixels that is either under or over corrected for the shading by the dark reference file.

Cures:

For some data, it is possible to fit a function to the affected column and add it back in as a delta bias, but the data in the affected pixels tends to be rather noisy as well. Given dithered data, you may be better off just treating the affected pixels as “bad” and using spatial dithers to recover that information (just as you would do for other bad pixels). Adding the middle column/row to the DQ array flags of the calibrated image (`*_cal.fits`), or to the MASKFILE before **calnica** processing, will mark them for exclusion when dithered images are subsequently combined by **calnicb** or **Multidrizzle**.

4.7.3 Coronagraphic Hole

NICMOS camera 2 includes a coronagraphic hole which can be used to partially obscure bright sources. In non-coronagraphic observations, however, the hole is still present, and will partially or completely blank out any objects which fall near it. For thermal IR images, the hole can appear as a positive “bump” due to excess background emission shining through the hole from warmer structures behind it. The position of the hole in detector coordinates has drifted with time, changing rapidly shortly after launch when the cryogen distortion of the dewar was varying quickly, then slowly stabilizing.

Cures:

The hole should usually be treated as “bad pixels” when combining dithered NIC2 images, either by masking or interpolation. Masking a circular region with radius ~ 7 pixels should eliminate the effects of the hole for most data sets. For coronagraphic imaging science, see the discussion on reducing coronagraphic data in Chapter 5.

4.7.4 Vignetting

There are two effects which are sometimes described as *vignetting* in the NICMOS cameras.

First, the anomalous expansion of the NICMOS dewar moved the cameras in such a way that they image the edge of the Field Divider Assembly (FDA) at the bottom of all 3 cameras. The FDA is a fold mirror that sends the light from the foreoptics down each camera channel and through the filters and dewar window to the cameras. The bottom edge of the field of view for all 3 cameras looks at a black mask on the FDA. This means that there is less signal from the telescope along that edge, and thus the throughput is decreased. In NIC3 ~15 rows along the bottom edge are severely affected, and the throughput there ramps down steeply to about 30% of the mean for the rest of the array. For NIC2 it has about the same extent, but is only reduced to 95% of the mean of the rest of the array. The effect for NIC1 is even smaller. This hard edge moves around slightly with time, and thus does not flat field away perfectly, especially for camera 3 where the gradient is steep. Because the vignetting is small for cameras 1 and 2, the resulting flat fielding uncertainty is generally negligible. (The coronagraphic hole in camera 2 is also on the FDA, so its motions correlate with those of the vignetted region.)

In addition, the NICMOS cameras also image part of the forward bulkhead at the entrance aperture. This warm metal surface emits radiation in the longer wavelength bands. This emission extends over about 50 rows in NIC3 and about 20 rows in NIC2. Moving the Field Offset Mechanism (FOM) causes NICMOS to see a different part of the sky in the *HST* focal plane, and essentially to look farther away from the bulkhead causing the emission. This FOM repositioning was automatically implemented for all NIC3 observations from January 1998 and onward, so data taken after that time are unaffected. Data in the longer wavelength filters taken prior to that time may have an elevated gradient in the sky background. The FOM is moved forward of the FDA in the optical path, so the repositioning has no effect on the FDA vignetting described above.

Another consequence of the vignetting is its impact on image shape and geometric distortion for NIC3 images. This concerns all data taken out of focus which is the case for all NIC3 data except data taken during the two refocus campaigns in January and June 1998 (no refocus campaigns have been conducted since the installation of NCS in 2002). The vignetting introduces some additional image distortion when the detector is out of focus, especially over the first ~50 rows of the detector (see e.g., Cox et al. Instrument Science Report OSG-CAL-97-07). Users should regard astrometry and PSF shape in that portion of NIC3 images with some caution.

Cures:

For NIC3, it may be prudent to discard data from the bottom 10 to 15 rows. At the very least, photometry in that region should be treated with suspicion. Data taken before the FOM repositioning in January 1998 may have elevated background gradients for NIC3.



For NIC3 images shape and astrometry over the bottom ~50 rows should be regarded with suspicion.


4.8 Effects of Overexposure

Because each pixel of the NICMOS detectors is read individually, overexposure does not cause “bleeding” along columns or rows, as is seen with CCDs. Sources that produce extremely large numbers of electrons in the detector, however, can result in two other sorts of NICMOS artifacts: persistent images, and electronic ghosts known colloquially as the “Mr. Staypuft” anomaly.

4.8.1 Photon Persistence

HgCdTe detector arrays are subject to image *persistence*. When pixels collect a large amount of charge, the photoelectrons are incompletely removed by reading the array and the remaining charge results in a signal on subsequent reads. This persistent signal decays exponentially with a time scale of about 160 ± 60 seconds, but there is also a long, roughly linear tail to the decay such that persistence from very bright sources remains detectable as much as 30 to 40 minutes after the initial exposure. Exposures of bright astronomical targets therefore can leave afterimages which appear in subsequent exposures taken within the same orbit, or even into the next (Figure 4.10). If you are analyzing dithered exposures of a bright target, you may wish to carefully inspect each image for residual ghosts from the previous exposure(s), and perhaps mask them out when co-adding the dithered images. It appears that all sources of photoelectrons leave persistent afterimages, but under typical conditions they are most noticeable for sources which have collected 20,000 or more ADU during the previous exposure. It is not unreasonable to expect afterimage signals of ~ 1 e^- /second immediately following a severe over-exposure. Occasionally, persistent images result from bright targets imaged by the *previous* NICMOS observer.

Figure 4.10: Persistence induced by an exposure of a bright star.

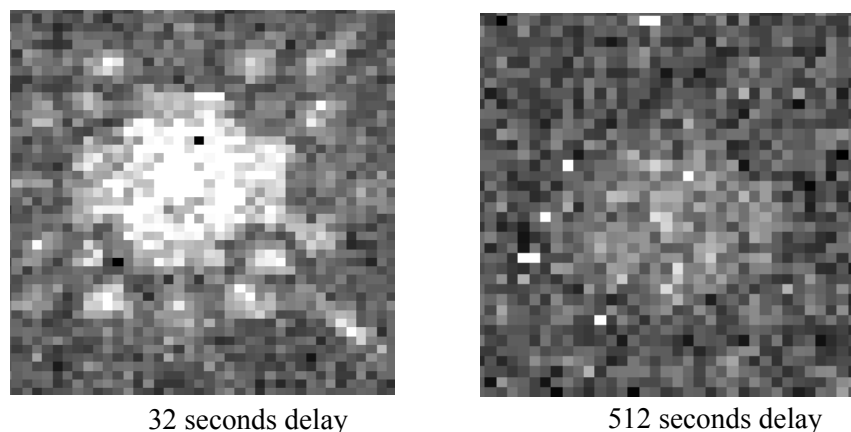

The left and right images show dark frames taken 32 and 512 seconds after the exposure of the star

Cures:

There is no easy cure for persistence in existing data; just be aware that it may be present. For dithered observations you can mask out persistent images from previous exposures before combining into a mosaic. It may be possible to subtract a rescaled version of the previous image that *caused* the persistent afterglow from the persistence image itself and thus remove it (see the discussion of cures for cosmic ray induced persistence below)


4.8.2 Cosmic Ray Persistence

More insidiously, during regular passages of *HST* through the South Atlantic Anomaly (SAA), the arrays are bombarded with cosmic rays, which deposit a large signal into nearly every pixel. The persistent signal from these cosmic rays may then be present as a residual pattern during exposures taken after the SAA passage. This appears as a mottled, blotchy or streaky pattern of “noise” (really signal) across the images, something like a large number of faint, unremoved cosmic rays. These persistent features cannot be removed by the MULTIACCUM cosmic ray processing done by the standard pipeline (i.e. the CRIDCALC step of **calnica**) because they are not transient. However, for data taken in Cycle 11 and beyond, a method for removing the persistence has been developed (**saaclean**) and it has been a part of the standard the pipeline since 2008. This method is further described under “cures” below and in Section 3.3.3

For Cycle 7/7N data and Cycle 11 and beyond data that has not been processed with **saaclean**, effects of cosmic ray persistence may affect image quality. The cosmic ray persistence adds non-Gaussian, spatially correlated noise to images, and can significantly degrade the quality of NICMOS data, especially for exposures taken less than 30 minutes after an SAA passage (see examples in Figure 4.11). Count rates from moderately bad cosmic ray persistence can be of order 0.05 ADU/second, with large

pixel-to-pixel variations reflecting the spatial structure of the signal. The effective background noise level of an image can be increased by as much as a factor of three in the worst cases, although 10% to 100% is more typical. This “noise” is primarily due to the spatially mottled structure in the persistence, not the added Poisson noise of the persistence signal itself. Because *HST* passes through the SAA seven or eight times a day, a large fraction of NICMOS images are affected by cosmic ray persistence to one degree or another. Observations of bright objects are hardly affected, since the persistent signal is usually quite faint. Similarly, short exposures are not likely to be badly affected because the count rate from persistence is low and may not exceed the detector readout noise. But deep imaging observations of faint targets can be seriously degraded. The NICMOS [ISR-98-001](#) (Najita, Dickinson and Holfeltz 1998) presents a detailed discussion of this phenomenon and its effects on imaging observations.

Figure 4.11: Cosmic Ray Persistence in Three Dithered NIC2 MIF1024 Images.

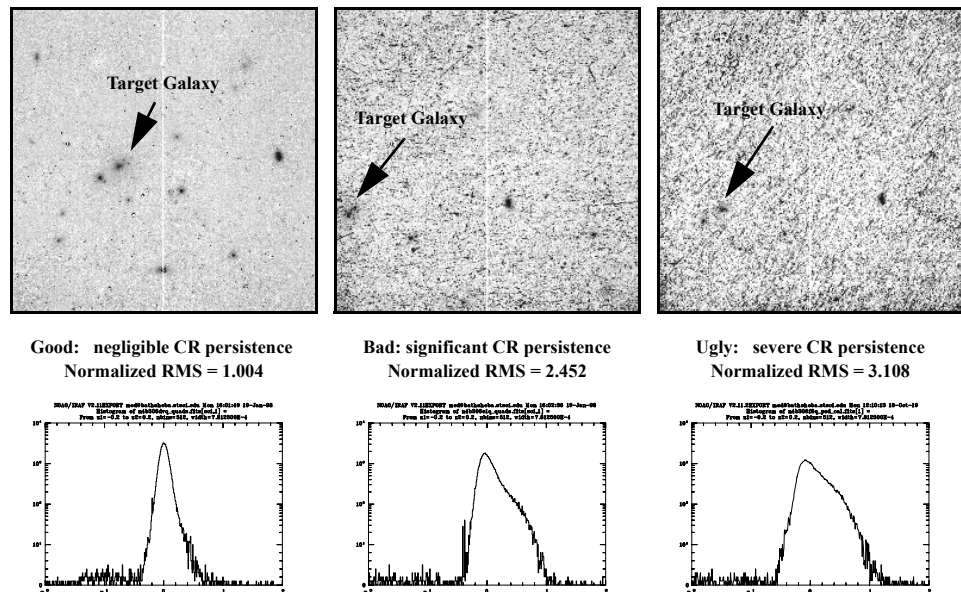

For each image, the histogram at bottom shows the distribution of pixel values near the sky level. The shoulder of positive values for the persistence-impacted images demonstrates the non-Gaussian nature of CR persistence noise. The “normalized RMS” is the measured value divided by the mean for many “clean” images free of CR persistence

Cures:

For Cycle 7/7N data there is no task to remove the persistence signal. However, if you have multiple exposures within a given SAA-impacted orbit, the amplitude of the persistence should decay, and you may want to give later exposures higher weight when combining them. Sometimes it may be preferable to discard the worst frames altogether. Well-dithered data lessens the impact of persistence, since objects will move relative to the persistent CR signal and it will not sum coherently when the data are registered. With well-dithered data (at least three positions), one can also

take advantage of the **MultiDrizzle** software to combine images after masking the persistence.

Starting in Cycle 11, the operating procedure has been to automatically perform a pair of ACCUM mode darks for each NIC camera following every SAA passage, provided there is a NICMOS observation scheduled before the next SAA passage. Post-SAA darks can be identified by the target name “POST-SAA-DARK.” **Calnicb** generates a product that is currently a simple average of the two dark exposures and the product filename is **ipppssoot_saa.fits**. The post-SAA dark exposures that are associated with a given observation are automatically retrieved with the science data whenever a post NCS NICMOS science observation is retrieved from the *HST* Archive.

Keywords **SAA_EXIT** and **SAA_TIME** contain information about the last exit from the NICMOS SAA contour. **SAA_dark** and **SAACRMAP**¹ contain information about the post-SAA dark that was taken closest in time to the science exposure. The values of the **SAA_EXIT** and **SAA_TIME** keywords are used by the OPUS pipeline to identify the filenames of the post-SAA darks closest in time to the respective NICMOS observation. These filenames are written into the header keywords. If no post-SAA dark is appropriate for a given science observation, the value of these keywords will be set to ‘N/A’. The new keywords are presented in the following example:

/POST_SAA DARK KEYWORDS

```
SAA_EXIT= '2000.171:12:34:49' /time of last exit from SAA contour level 23
SAA_TIME= 1529 /seconds since exit from SAA counter level 23
SAA_DARK='N/A' /Association name for post-SAA dark exposures
SAACRMP='N/A' /SAA cosmic ray map file
```

The NICMOS team has developed and tested a **PyRAF** task (based on the original algorithm developed by L. Bergeron) called **saaclean** (see Section 3.3.3) that utilizes post-SAA darks in order to remove cosmic ray persistence. This task is delivered with **STSDAS** version 3.6 and located in the **stsdas.hst_calib.nicmos** package of **PyRAF** version 1.3 or later. Starting March 31, 2008 the **saaclean** task is included in the OTFR, therefore all data retrieved from the archive after that date will have the SAA cosmic ray persistence removed. For more information, please see the NICMOS [ISR 2007-001](#) by Barker, Laidler, and Koekemoer, and the task help file. The original detailed algorithm and IDL software tool developed by L. Bergeron are described in Both the algorithm and the tool are described in NICMOS ISR by Bergeron and Dickinson (2003, NICMOS [ISR 2003-010](#)).

1. The SAACRMAP keyword is no longer being used by the OTFR pipeline

4.8.3 Bright Earth Persistence (BEP)


It has recently been found that the NICMOS detectors may be exposed to another type of persistence, Bright Earth Persistence (BEP). This occurs in rare instances when HST is pointed towards the bright earth and one or more of the NICMOS filter wheels are not yet in the blank position. The result is an effect similar to that encountered during SAA passages, image persistence with multiple trap decay time scales, but with a different source of excitation, soft photons instead of cosmic rays. The persistence image resulting from exposure to the bright earth is similar in appearance to the persistence resulting both from intense cosmic rays and from using onboard lamps. However, the bright earth exposes the detectors more evenly than in the case of cosmic rays and more intensely than from the onboard lamps. The procedure used for removing cosmic ray persistence therefore needs to be modified to account for this. A description of the BEP effect and an outline of how it can be removed is given in NICMOS [ISR 2008-001](#) (Riess & Bergeron 2008). For further updates please refer to the NICMOS Web page at:

<http://www.stsci.edu/hst/nicmos>

The occurrence of BEP depends on several factors and it is currently not known to what extent NICMOS data is affected. It is likely to be a fairly small fraction, but large enough to require a cure (see below). In order to avoid exposing the detectors to the bright earth, each NICMOS filter wheel will normally place the blank in front of the detectors whenever the HST is pointing within 20° of the earth's bright limb (and 6° from the earth's dark limb). However, if NICMOS is operating in parallel with another instrument, the read-out of this instrument will take precedent and could, in rare circumstances, lead to a delay in moving the NICMOS filter wheel.

The combination of ACS as primary and NICMOS as parallel instrument is known to have resulted in BEP in NICMOS. Another instance that could result in exposure to the bright earth is if a slew is initiated immediately following a NICMOS visit and this visit ended before reaching the Earth Avoidance Zone. The telescope will then be slewing, possibly across the bright earth, while the NICMOS filter wheels are in motion.

Figure 4.12: NIC2 Persistence Images

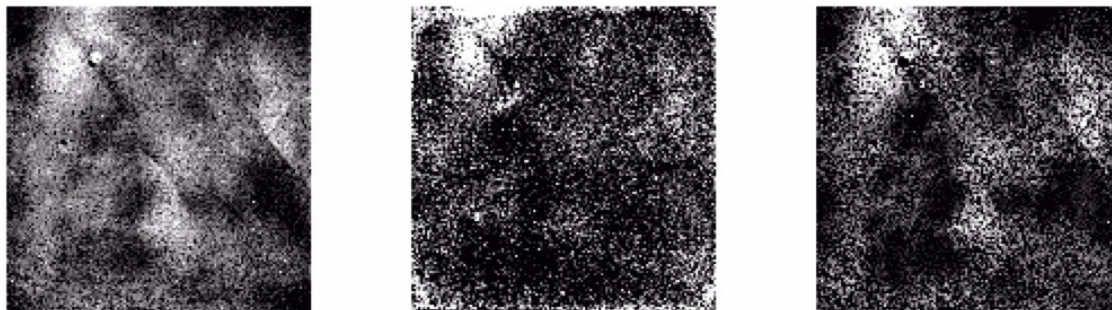

The far left is the BEP image derived from the 10 impacted visits of the SHOES program. The middle panel is the persistence seen from the scattering of the full detector by CR hits in numerous SAA passages. The version on the right, like SHOES, is caused by persistence from photons, in this case after the use of the lamps. The best signal-to-noise ratio for modeling the persistence comes from the BEP on the left due to its more uniform and greater excitation.


Cures:

Removal of the BEP is done in a manner similar to the removal of cosmic ray induced persistence from SAA passages. A stored BEP persistence image is scaled to the measured persistence and subtracted from the science image. This procedure is repeated until less than 50% of the background pixels are affected. This rather high limit is set to avoid affecting sources in the image. Due to the large coverage of afflicted pixels, the scaling is done by minimizing the residuals relative to a flat sky (without sources). In contrast, SAA cosmic ray persistence is scaled by minimizing residuals relative to adjacent pixels because of the quantized "illumination" by the random cosmic ray hits. For more details about the routine, `nic_rem_persist` that removes BEP, please refer to Section 3.3.3

4.8.4 Amplifier Ringing (The “Mr. Staypuft” Anomaly)

There is another sort of NICMOS ghost image, wholly separate from those induced by persistence. Bright targets which appear in a given detector quadrant can produce an electronic *ringing* effect in the readout amplifiers, which may induce ghost images at the same pixel locations in the other three quadrants. This is believed to be due to the pull-down of the power supply, which does not completely recover from reading a large number by the time it’s asked to read the next number (from the next quadrant). In some cases a whole row (or column, whichever direction the “fast” read clocking runs) can be anomalously high. The amplitude of the ghost images is of order a tenth of a percent of the real image count rate. Inside the STScI NICMOS group, this effect is fondly known as the “Mr. Staypuft anomaly” (Figure 4.13).

Figure 4.13: The Mr. Staypuft Anomaly.

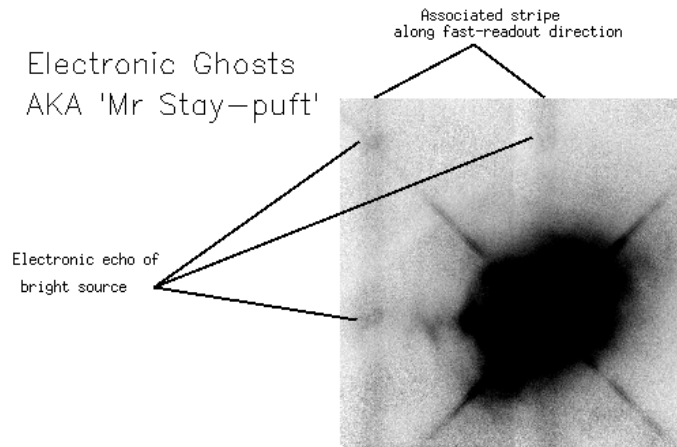

The bright source at lower right produces electronic ghost images in the other three quadrants, plus vertical streaks. In Camera 1 images, these streaks run horizontally

Cures:

The STScI NICMOS group has developed the **STSDAS "puftcorr"** task which identifies and removes the Staypuft column/row effect in post-processing, based on an empirical model for its electronic behavior. For example, if your image has a bright source at pixel (58,143), then you may see ghost images around (186,143), (186,15), and (58,15). If the observation was made with Camera 3 (so that the fast clocking direction is along columns), there may also be elevated signal at all rows on and around columns 58 and 186. Ordinarily it is not possible to eliminate these ghosts from dithered data by masking, since they will move about on the array along with the astronomical targets. If, for some reason, observations were obtained at multiple roll angles, then it would be possible to mask the ghosts and eliminate them; this was done for the Hubble Deep Field South NICMOS observations.


Some NICMOS observers studying relatively blank fields have dealt with the “elevated columns/rows” phenomenon by fitting medians to the affected columns/rows (or to portions of the columns/rows, avoiding regions affected by bright or extended targets), and subtracting the median values from each column or row of the data. This can at least provide a cosmetic fix. In principle, this correction should probably be applied *before* flat fielding the images, since it is most likely that the “Staypuft” signal is not responding to the array QE variations, although this has not yet been formally tested. However, if the fit is done before flat fielding, then the sky background itself will not be uniform, and in fact will be improperly subtracted by the procedure. For this reason, in practice it is probably safer

(if not strictly correct) to apply a median column (or row, for NIC1) correction after flat fielding instead. For updates, please refer to the [NICMOS Electronic Ghosts Web](#) page.

4.8.5 Optical Ghost Images

In addition to persistence and electronic ghosts, NICMOS polarimetric images of bright targets are subject to optical ghosts (Figure 4.14). These are most evident for the short wavelength polarizers in NIC1. The location of the polarizer ghosts relative to the source changes direction with respect to the principal axes of transmission. For POL0S, the brightest ghost is found roughly $(-10,+35)$ pixels away from the target position, and a second one at $(-16,+70)$ pixels. It is possible that for a brighter object more ghosts would appear in the same angle and direction. POL120S images appear to be ghost-free. For POL240S, ghosts appear $(+10,+54)$ pixels from the source position and $(+18,+80)$ pixels, with the possibility of more appearances for brighter targets.

Figure 4.14: Optical ghosts in NIC1 polarizers.

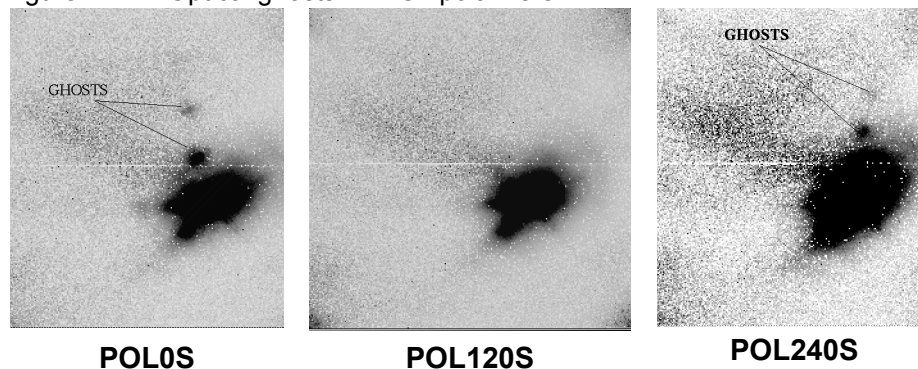

Ordinary (non-polarimetric) NICMOS images of bright sources may have very faint filter ghosts which result from back-reflections off the faceplate and the filters. The position of the ghosts changes from one filter to another. They are roughly 8 magnitudes fainter than the star which produces them. The ghosts cannot be completely subtracted from the field unless the reference PSF is at the exact same location as the star. They are typically seen as a residual in the PSF subtracted images, and look like large “donuts” because they are out-of-focus reflected images.

Cures:

No true cure is possible: be aware that such ghosts may exist; their positions are predictable. If images are available with multiple spacecraft roll angles, the ghosts may be masked out before combining the data.

4.9 Cosmic Rays of Unusual Size


As with CCDs, cosmic ray (CR) hits produce unwanted signal in the output images. Unlike standard CCD observations, however, most of the effects of CRs in NICMOS data can be eliminated during data processing thanks to the capability for multiple, non-destructive readouts in infrared arrays. As was described in Chapter 3, the **calnica** processing pipeline identifies cosmic rays in individual readouts of a MULTIACCUM image during the CRIDCALC step, and excludes data from that readout when calculating the final count rate for the affected pixel. Therefore CRIDCALC processed NICMOS images (`*_cal.fits`) should be free of most or all ordinary cosmic rays. The affected pixels will be flagged in the DQ extensions of the `*_ima.fits` files.

It is worth noting that the noise level will be slightly higher for pixels which were impacted by cosmic rays because (1) the effective exposure time for those pixels is shorter because one readout has been discarded, and (2) breaking the counts vs. time “ramp” fitting procedure into two or more pieces introduces extra statistical noise, particularly for observations limited primarily by readout noise.

Images taken in ACCUM mode have no cosmic ray processing. For these, you must handle cosmic rays as you would for ordinary CCD images.

Occasionally NICMOS (like other instruments) will be hit by a very strong cosmic ray, that can affect many pixels (Figure 4.15). These will not always be effectively removed by the **calnica** CRIDCALC processing. The core of the very bright CR will be flagged and removed, but there can be a large, surrounding “halo” of pixels weakly affected by CR signal that are not flagged. Also, glancing-incidence cosmic rays can leave long trails across an image, and the weaker CR pixels in the streak may not be flagged by the CRIDCALC processing. Very strong CRs can induce persistence which will alter the count rate for the rest of the MULTIACCUM sequence, resulting in a cosmic ray afterimage. If pixels reach saturation levels from a cosmic ray impact, subsequent readouts are unrecoverable.

Figure 4.15: A “Monster Cosmic Ray” Hit in a NICMOS Image.

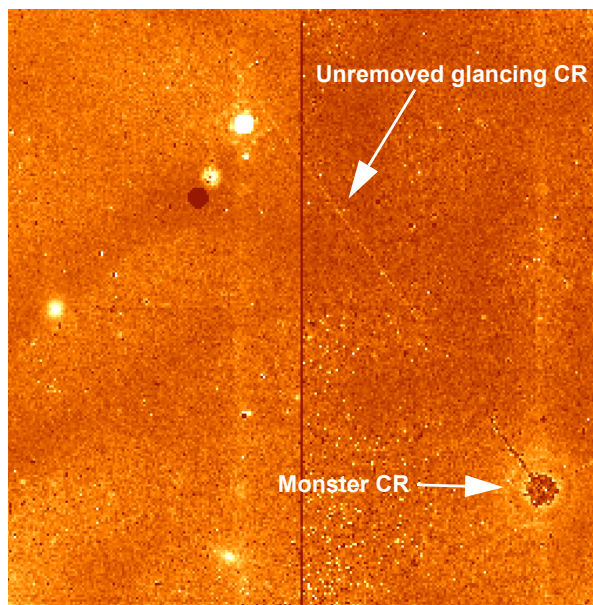

The brightest pixels of the CR have been cleaned by CRIDCALC in **calnica**, but a surrounding halo of affected pixels remains, as does a long diagonal streak of unflagged pixels from the CR’s glancing traversal of the array. Also note the vertical “Mr. Staypuft” streaks (see Section 4.8.4) in both the left and right halves of the image, which are evidently induced by the CR impact itself.

Cures:

If weakly affected pixels around bright cosmic rays are not being flagged by CRIDCALC, you may wish to reprocess the data, reducing **calnica**’s CR rejection threshold parameter *crthresh* from the default (4) to a smaller value. Alternatively, you may flag the cosmic ray affected pixels manually before CRIDCALC processing. First, partially process the images through **calnica** excluding the CRIDCALC stage (i.e. setting CRIDCALC to OMIT). Next, in the resulting **_ima.fits* image, edit the DQ extension of the first IMSET affected by the cosmic ray, setting the affected pixels to the cosmic ray flag value 512 (see Table 2.3). Finally, set CRIDCALC to PERFORM in the **_ima.fits* file and complete the **calnica** processing using the modified **_ima.fits* as input.



The technique described here for flagging monster cosmic rays can also be used to flag and eliminate trails from moving targets (usually space junk) which occasionally cross through NICMOS images.

4.10 Scattered Earthlight

All *HST* instruments are occasionally subject to scattered earthlight which enters when the telescope is pointing near the bright earth limb. This results in an elevated background level, which does not necessarily illuminate the detector in the same way as the sky does, and thus does not flat field away properly. For NICMOS MULTIACCUM observations, scattered light during a portion of the exposure (usually either the beginning or the end) will also cause the signal level to accumulate in a non-linear way with time, i.e. either with an initial or final “ramp-up” where the scattered light elevates the count rate for some of the readouts. This can cause problems when the **calnica** CRIDCALC routine fits a linear function to counts vs. time, triggering the rejection algorithm for some pixels and not others, and resulting in erroneous slope fits (and hence, incorrect derived count rates) for some pixels.


Cures:

Fortunately, for a MULTIACCUM observation, one can take advantage of the time resolved nature of the data to exclude individual readouts where scattered light contaminates the data. As an example, let us look at one data set where scattered light plays a role. In this example, we will also use some of the tools in the **stdas.hst_calib.nicmos** package which are described in more detail in Chapter 5. First, we will partially process the image through **calnica** using **nicpipe**, skipping the UNITCORR, FLATCORR and CRIDCALC steps. The resulting *_ima.fits image is thus in units of counts, not countrate. Next, we use the **sampdiff** task to plot the median counts in each IMSET of the image vs. the sample time.

```
ni> nicpipe n4ux11ufq_raw.fits "" stage=biaseq
ni> pstats n4ux11ufq_ima.fits \
>>> extname=sci units=counts stat=midpt
```

The result is shown in Figure 4.16:

Figure 4.16: Plot of median counts vs. time for readouts from a NICMOS image.

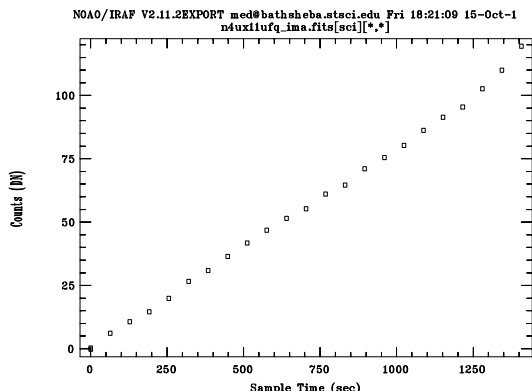


The upturn in the last few readouts shows the effects of scattered light

The upturn in the counts during the last few readouts indicates the presence of scattered light at the end of the exposure. It is sometimes easier to see the effects of scattered light if you look at the “first differences” in an image, i.e., the *difference* between each readout and the preceding one. In that way, you see only the counts that were accumulated during that readout sample, and not the cumulative sum of everything that came before. This can be done using the task **sampdiff** in the **nicmos** package (again, see Chapter 5).

```
ni> sampdiff n4ux1lufq_ima.fits n4ux1lufq_fdiff.fits
ni> pstats n4ux1lufq_fdiff.fits \
>>> extname=sci units=counts stat=midpt
```

Figure 4.17: Scattered light with difference.

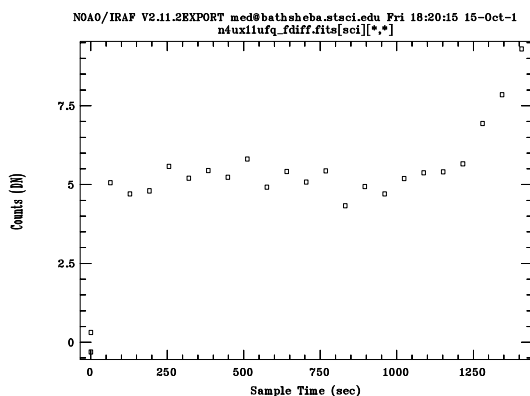

Median counts per IMSET for the “first difference” image computed from the *_ima.fits file using **sampdiff**. The upturn due to scattered light is more prominent when viewed this way.

The easiest and safest way to eliminate the effects of scattered light is to discard the affected readouts before fitting with CRIDCALC to compute the count rates and identify the cosmic rays. This will cost you part of the exposure time in your image, but will eliminate the elevated background, the uneven illumination, and problems resulting from incorrectly fit count rates and accidental triggering of the CRIDCALC cosmic ray rejection. This can easily be done by editing the data quality arrays in the DQ extensions of the affected images, setting them to some non-zero value (8192 is a good choice, as it is not otherwise used as a DQ flag value for NICMOS). This will cause CRIDCALC not to use those imsets when fitting a slope to counts vs. time to derive the count rate. You can edit these in the raw data frame and start over with the processing, or (in the example we are using here) in the partially processed frame, and then complete the processing using **nicpipe**. For our example, we might continue in the following way. We want to exclude the last three readouts from further processing. Remember that NICMOS imsets are stored in reverse order in the multiextension FITS file, i.e., [SCI,1] is the last readout, [SCI,2] the next to last, etc.

```
ni> copy n4ux11ufq_ima.fits n4ux11ufq_imaflag.fits
ni> imreplace n4ux11ufq_imaflag.fits[DQ,1] 8192 ver- up+
ni> imreplace n4ux11ufq_imaflag.fits[DQ,2] 8192 ver- up+
ni> imreplace n4ux11ufq_imaflag.fits[DQ,3] 8192 ver- up+
ni> nicpipe n4ux11ufq_imaflag.fits "" stage=final
```

The end product will be called `n4ux11ufq_imaflag_cal.fits`, and should be free of scattered light, albeit with a somewhat shorter effective exposure time. The actual exposure time used per pixel can be determined by looking at the [TIME,1] array of the final, calibrated image.

Data Analysis

In this chapter. . .

5.1 STSDAS Software / 71
5.2 Photometric Calibrations / 76
5.3 Astrometry, Pixel scales, and Geometric Distortion / 89
5.4 PSF Subtraction / 93
5.5 Coronagraphic Reductions / 100
5.6 Analysis of Polarization Images / 114
5.7 Grism Data Reduction / 119

5.1 STSDAS Software

Software tools for NICMOS FITS files available in the **STSDAS** packages. **toolbox.imgtools.mstools** and **hst_calib.nicmos** have been designed to maintain compatibility with pre-existing analysis software. The tools have either been written in ANSI-C or are **IRAF** CL scripts interfacing with pre-existing **IRAF/STSDAS** tasks.

These tasks include tools for mathematical and statistical operations on science images and for analysis and display of reduced and raw data. In most cases, the utilities extend existing routines to include error and data quality propagation. These are the utilities of greatest interest to the user community. Under this category are several tasks described in Chapter 3 of the "[HST Data Handbook](#)", **msarith**, **mscombine**, **msstatistics**, **msjoin** and **mssplit**, along with a few other tasks we describe below, **ndisplay**, **markdq**, **mosdisplay**, **pstack**, **pstats**, **sampinfo**, **sampdiff**, **sampcum**, **CalTempFromBias**, **puffcorr**, **nicpipe**, **biaseq**, **pedsky**, **pedsub**, **saaclean**, **nic_rem_persist** and **rnlincor**. The first five are found in the package **toolbox.imgtools.mstools**; the remaining ones reside in the package **hst_calib.nicmos**.

The tasks in the **toolbox.imgtools.mstools** package are particularly useful for working with individual STIS and NICMOS imsets. See

“Working with STIS and NICMOS Imsets” in Chapter 3 of the ["HST Data Handbook"](#) if you are not familiar with these tasks. Below we describe a few tasks of specific interest to NICMOS observers. For additional details and examples of these and other tools, please refer to the online help.

There used to be a package called **nicproto** for new experimental software that was released between major **STSDAS** releases. This package was removed in 2000 and was superseded by placing new tasks in the **nicmos** package in regular **STSDAS** releases only. All routines described in this edition of the handbook are available in **STSDAS** versions v3.9 and later.

ndisplay and markdq

The **markdq** task reads the data quality (DQ) array from a NICMOS image and marks the DQ flags on the displayed image. Each flag value can be set independently to a different color or can be turned off. The **ndisplay** task combines the capabilities of the **IRAF** task **display** and the task **markdq**: it displays a NICMOS image and overlays the DQ flags according to a user-specified color-code. Both tasks are useful for locating specific DQ values, for example, the cosmic rays rejected by **calnica** in a MULTIACCUM image.

mosdisplay

The **mosdisplay** task provides a convenient way to display images from all IMSETS of a NICMOS MULTIACCUM image together as a mosaic in a single ximtool or saimage window. The user may select which extension (e.g., SCI, ERR, TIME, SAMP, or DQ) to display, and can control the display threshold parameters or leave them to be automatically determined.

pstack and pstats

The **pstack** and **pstats** tasks plot all the samples of a specified pixel or image section, respectively, from a NICMOS MULTIACCUM image as a function of time. These tasks can be used to track the time behavior of an image on a pixel-by-pixel basis. For example, the temporal positions of cosmic ray hits or the onset of saturation during the course of an exposure can be located for a defined set of pixels. The **pstats** task can be particularly useful for identifying anomalous data behavior such as drifting bias levels or scattered light which may cause the background level to vary substantially during the course of an exposure.

sampinfo

The **sampinfo** task offers a convenient way to get readout-by-readout information about a NICMOS MULTIACCUM image. It provides information about the overall readout sequence (SAMP_SEQ, NEXTEND, NSAMP, and EXPTIME), and then for each imset of the multi-extension fits file it lists the corresponding SAMPNUM, SAMPTIME and DELTATIME values. These can be useful bits of information when using

non-standard processing techniques, such as the **biaseq** routine. An example of the use of **sampinfo** and its output is given in Section 4.2.4.

sampdiff and sampcum

The **sampdiff** task provides a convenient way to convert a MULTIACCUM image into a set of independent “first differences.” Normally, each IMSET (readout) of a MULTIACCUM image is the cumulative sum of the total exposure time prior to that readout. As such, the `[sci,*]` images are not statistically independent. When analyzing NICMOS images, it is sometimes helpful to look at the data which was collected during each readout interval independent of that which was accumulated previously, i.e. by taking the difference of successive readouts. In this way, you can isolate readouts with problems (e.g., major cosmic ray hits or moving objects, sudden changes in bias, scattered light, etc.). The **sampdiff** task automates this process. *Note that, in general, this is only really a sensible thing to do if the image has not been converted from counts to count rate by the UNITCORR step of calnica!* The **sampcum** task inverts this process, re-accumulating the first differences.

CalTempFromBias

This routine calculates the temperature of the detector from the measured bias levels. This routine works only on MULTIACCUM observations and runs on the `*_raw` files. This routine needs to be run before **calnica** such that an accurate temperature of the detector is determined that allows the right reference files to be used for dark subtraction, flat fielding, and photometric sensitivity correction. Details of this routine can be found in Section 3.3.1

Puftcorr

The **puftcorr** task measures and removes an estimate of the “Mr. Staypuft” anomaly or quadrant crosstalk signal in a NICMOS image. This correction is only needed if there are bright sources in the image. The input image to the task must be a `*_raw` MULTIACCUM NICMOS dataset, with no **calnica** processing yet applied. The effect is described in more detail in Section 4.8.4.

nicpipe, biaseq, pedsky and pedsub

The **nicpipe** task provides a shortcut for partially processing NICMOS images through some but not all stages of **calnica**. Normally, this is meant for use in preparing images for “bias equalization” using the **biaseq** task (see Chapter 4). Setting `stage=biaseq` takes the processing through the steps **ZSIGCORR**, **ZOFFCORR**, **MASKCORR**, **BIASCORR**, **NOISCALC**, **DARKCORR**, **NLINCORR**, and **BARSCORR**. Setting `stage=final` completes the processing. This can also be done by hand using **chcalpar** or **hedit** to change the processing control switches in the image headers (see Section 3.5.2) and running **calnica** directly.

Occasionally **nicpipe** can come in handy at other times besides **biaseq** processing: one example is given below.

The tasks **biaseq**, **pedsky**, and **pedsub** provide methods for dealing with the floating quadrant bias or “pedestal” effect in some (not all) data sets, and are described in Section 4.2.4.

Saaclean

The **saaclean** task measures and removes an estimate of the SAA persistence signal in a NICMOS image. **Saaclean** runs on a single science image (i.e., not on all the separate readouts of a NICMOS MULTIACCUM file). It is generally recommended that the images have gone completely through **calnica** and have been processed by **pedsub** as well. The routine uses post-SAA darks, which were only taken automatically since Cycle 11 in the post-NCS era. **Saaclean** is part of the **runcalsaa** software and is included in the OTFR since March 2008. More details about this SAA persistence routine can be found in Section 3.3.3 and in the routine’s help file.

nic_rem_persist

The **nic_rem_persist** routine removes the persistence of the bright Earth that may have been falling on the detector during the previous occultation when operating NICMOS in parallel with another instrument. This will leave a large scale noise pattern that is slowly declining. **nic_rem_persist** is part of the **runcalsaa** software and is included in the OTFR since March 2008. Further information about this effect and this routine can be found in Section 3.3.3.

rnlincor

The **rnlincor** task corrects for the countrate-dependent nonlinearity in a NICMOS image. The input image to the task must be a NICMOS science image in units of DN/s that has been processed through **calnica**, and preferably has also been corrected for pedestal with either the **pedsky** or **pedsub** tasks. As the countrate nonlinearity is assumed to depend on incoming flux/countrate, the image should have instrumental effects removed as much as possible. Grism and polarimetry images are not supported by this task. Details about this countrate nonlinearity routine can be found in Section 4.5 and in the help file.

Using These Tasks: An Example.

As an example, you might want to inspect NICMOS data for anomalies which occur during individual readouts during a MULTIACCUM using a procedure like this:

```
ni> nicpipe n4xj13jwq_raw.fits "" stage=biaseq
ni> sampdiff n4xj13jwq_ima.fits n4xj13jwq_fdiff.fits
ni> mosdisplay n4xj13jwq_fdiff.fits 1 extname=sci number+
ni> pstats n4xj13jwq_fdiff.fits[1:128,1:128]\
>>> extname=sci units=rate stat=midpt
```

In this example, the raw image is first partially processed through **calnica** using **nicpipe**. By setting `stage=biaseq`, the pipeline processing stops before flat fielding, conversion to count rate, and CRIDCALC cosmic ray processing. You then take first differences with **sampdiff**, displays them as a mosaic with **mosdisplay** to look for bars, bias jumps, monster cosmic rays, or other oddities in individual readouts, and then use **pstats** to plot the median count rate (`units=rate`) per sample time in the image quadrant `[1:128,1:128]`.

Having satisfied yourself that the data is fine, you might then complete processing using the **biaseq** and **pedsky** tasks in the following manner:

```
ni> biaseq n4xj13jwq_ima.fits n4xj13jwq_beq.fits \
>>> skysamps=1-13 fitbias+ fitjump+
ni> nicpipe n4xj13jwq_beq.fits "" stage=final
ni> pedsky n4xj13jwq_beq_cal.fits n4xj13jwq_ped.fits \
>>> salgorithm=auto interactive+ rmedian-
```

In this case, you have corrected readout-to-readout bias drifts with **biaseq**, also fitting for bias jumps in the process, and then carried out the final “pedestal” correction with **pedsky**, solving for the background level and pedestal interactively. Please see Section 4.2.4 of this manual and the on-line help files for **biaseq** and **pedsky** for a detailed explanation of the parameters. The resulting end product image will be `n4xj13jwq_ped.fits`.

5.2 Photometric Calibrations

Atmospheric absorption bands limit the wavelength ranges over which one can usefully observe in the near-infrared from ground-based telescopes. NICMOS, however, can observe at any wavelength where its detectors are sensitive, and hence its filter bandpasses do not conform to those of instruments used at ground-based observatories. Instead, its filters were designed to meet the anticipated scientific demands. Thus in practice NICMOS does not have filters matched to any of the ground-based photometric bands and calibration has to be performed independently. The photometric calibration of NICMOS data is discussed in this section. Cases of continuum sources, emission lines, and grism spectra will be presented.

5.2.1 Units for NICMOS Photometry

Given the multitude of units and systems that have been used for infrared photometry (magnitudes, Jy, $\text{W m}^{-2} \mu\text{m}^{-1}$, $\text{erg sec}^{-1} \text{cm}^{-2} \mu\text{m}^{-1}$, etc.) and given the lack of a standard for ground-based infrared filters, NICMOS has adopted the approach of calibration to physical units, i.e. Janskys (Jy), or Jy arcsec^{-2} for surface brightness. Details on how to transform different sets of units can be found in Appendix B of the *NICMOS Instrument Handbook* or obtained using the [NICMOS Unit Conversion Tool](#) (available on the STScI [NICMOS Web](#) pages).

5.2.2 Fluxes and Magnitude Zeropoints

The NICMOS calibration pipeline provides two photometric parameters for the conversion of countrates into fluxes. These parameters are found in the keywords PHOTFNU and PHOTFLAM in the header of the calibrated image. The definitions of these keywords are discussed in Section 3.4.4 of the "[HST Data Handbook](#)". Very briefly, for NICMOS these are the bandpass-averaged flux densities (in F_λ for PHOTFLAM or F_ν for PHOTFNU) for a source that would produce a count rate of 1 DN sec^{-1} . PHOTFNU is given in units of Jy sec DN^{-1} and PHOTFLAM in units of $\text{ergs cm}^{-2} \text{\AA}^{-1} \text{DN}^{-1}$. Because NICMOS calibrated data are given in countrate, i.e., DN sec^{-1} , the countrate to flux conversion is simply achieved by multiplying the countrate by the PHOTFNU or PHOTFLAM value, depending on which units are desired for the final calibrated image.

A fundamental challenge in calibrating NICMOS photometry is the inherent uncertainty in absolute flux calibration in the near-infrared, whether from the ground or from space. Unlike the situation at optical wavelengths, there really are no absolutely calibrated spectrophotometric flux standards at near-infrared wavelengths. Ground-based photometric

calibration observations are mostly limited to relative magnitude determinations in more or less standard bandpasses (*JHK*) defined by atmospheric absorption windows. But the absolute flux calibration of primary infrared standards has generally been based on reference to some assumption that a particular type of standard star, e.g., solar-type stars, A0 stars, or white dwarfs, has a spectrum similar to something else that is believed to be well understood, such as the Sun or a well-calibrated stellar atmosphere model. As an example, see Campins, Rieke & Lebofsky (1985), who used the solar analog approach to derive absolute flux calibrations in the near-infrared. These calibrations are uncertain at a level of several percent, setting a fundamental limit on the accuracy of any absolute flux calibration in the near-infrared, including that of NICMOS.

In the case of NICMOS, the photometric calibration is based on observations of solar analogs and hydrogen white dwarfs (WDs). The stars P330E (solar analog) and G191B2B (WD) define the primary calibration, with a few other stars observed as cross-checks. Bohlin (2006, astro-ph/0608715) recalibrated the absolute flux density distribution of the *HST* NICMOS standards. The UV, optical and near-IR portions of their spectra were measured with high quality *HST* STIS and NICMOS grism observations. These were then carefully matched to stellar atmosphere models to correct for the NICMOS nonlinearity and for extrapolation to near-infrared wavelengths not covered by the grism observations. The absolute calibration of these spectra are now thought to be accurate at the 2-4% level, the relative errors within the spectra are at the 1-2% level (Bohlin, 2007, ASPC, 364, 315)

The STScI NICMOS group has reanalyzed all photometric calibration data taken in orbit with NICMOS during Cycles 7, 7N, 11 through 15. For further updates please refer to the NICMOS Web page at:

<http://www.stsci.edu/hst/nicmos>

as well as interim sets of calibrations presented in earlier editions of the handbook. Unlike earlier efforts, the new work uses a larger number of measurements, applies uniform and up-to-date NICMOS calibration software and reference files, and employs a more careful treatment of the NICMOS photometric aperture corrections¹ (See “Aperture Correction” on page 85.) than was used for the original calibration efforts. The current best estimates of the `PHOTFNU` and `PHOTFLAM` values for NICMOS filters can be found on the NICMOS photometry Web page at:

<http://www.stsci.edu/hst/nicmos/performance/photometry>

1. The `PHOTFNU` and `PHOTFLAM` keywords represent photometry corrected to infinite aperture, i.e., the scaling between stellar flux density and the *total* count rate measured from a star within a (hypothetical) infinite aperture. The actual standard star measurements are made within a fixed, finite radius aperture and corrected to infinite aperture using mode point spread functions from **TinyTim**. The apertures and corrections used for the different filters are listed in the post-NCS photometric tables.

These new values update previous numbers given in older versions of the PHOTTAB calibration reference files, as well as an interim set of calibrations presented in an earlier edition of this *Handbook* (version 4.0). The new calibrations are believed to be accurate to better than 5%, thus satisfying the absolute calibration requirements for NICMOS. For most filters, the *relative* calibration accuracy should be better, <3%, with the possible exception of some narrow band filters where uncertainties in absorption line strengths for the solar analog and white dwarf models may result in greater calibration errors. The PHOTFNU and PHOTFLAM values listed in the photometric keyword tables are the error-weighted averages determined from the P330E and G191B2B calibration stars. The listed fractional error was determined from the individual uncertainties in the determination of both stars and their RMS difference. It does not include the uncertainty of the absolute calibration of the reference spectra, which is believed to be less than 2-4%.

Please note that the NIC1 and NIC2 polarizers have not yet been recalibrated. The values given in the [pre-NCS photometric keyword tables](#) are taken from the older PHOTTAB calibration reference file `i7112297n_pht.fits`. Likewise, the polarizer values in the [post-NCS photometric keyword tables](#) were derived from the old Cycle 7 values, only correction for the change in sensitivity due to the higher operating temperature during post-NCS. Note also that the photometric calibration for the extremely broad band filters F140W, F150W and F175W should be used with caution. These bandpasses are so broad that the conversion from source flux to count rate will be very strongly dependent on the color or spectrum of the source.



We list photometric zeropoint tables for both the pre- and post- NCS eras. The higher operating temperature of the detectors after installation of NCS has significantly increased their sensitivity (15-70% depending on wavelength), which is reflected in the calibration zeropoints. The post-NCS calibration values were not available before the summer of 2004, and any data retrieved from the archive before this time will have incorrect calibration keywords in their headers.

In the header of calibrated NICMOS images, there are three additional photometric parameters that characterize the filter used for the observation (PHOTPLAM and PHOTBW) and provide the ST magnitude zero point (PHOTZPT). PHOTPLAM gives the value of the pivot wavelength of the

filter in Angstroms. This wavelength is source-independent and is the wavelength for which:

$$PHOTFLAM = c \times PHOTFNU \times PHOTPLAM^{-2}$$

where c is the speed of light in vacuum. $PHOTBW$ gives the rms band width of the filter in Å (see the [Synphot User's Guide](#) for a detailed definition of both parameters).

The magnitude of an object can be determined in the ST system (e.g., based on a constant flux per unit wavelength) using the photometric zeropoint keyword $PHOTZPT$ (= -21.1) simply by:

$$\begin{aligned} m_{ST} &= -2.5 \log(PHOTFLAM \times CR) + PHOTZPT \\ &= -2.5 \log(PHOTFLAM \times CR) - 21.1 \end{aligned}$$

where CR is the count rate in units of DN sec⁻¹. On the other hand, the magnitude in Oke's AB_v system (e.g., based on a constant flux per unit frequency) is obtained by applying the following expression:

$$\begin{aligned} m_{AB} &= -2.5 \log(10^{-23} \times PHOTFNU \times CR) - 48.6 \\ &= -2.5 \log(PHOTFNU \times CR) + 8.9 \end{aligned}$$

As noted above, the NICMOS filter bandpasses do not match those of ground-based filters, and therefore it is not straightforward to derive “standard” infrared magnitudes normalized, e.g., to the spectral energy distribution of Vega. However, it may sometimes be useful to approximate a Vega-based photometric system by using an estimate of the flux density of Vega through the NICMOS bandpasses as a photometric zero point. Because there are no direct spectrophotometric observations of Vega or other A0V standards through the NICMOS filter system, our best option is to use a spectrophotometric model for Vega and synthetically integrate it through the bandpasses. [The photometric keyword tables](#) give bandpass averaged flux densities (in Jy) for the NICMOS filters using a model reference spectrum of Vega (Bohlin 2007, ASPC, 364, 315) available as `alpha_lyr_003.fits` in the database at STScI. An approximate Vega-normalized magnitude may be computed as

$$m = ZP(\text{Vega}) - 2.5 \log(PHOTFNU \times CR \times \langle F_v(\text{Vega}) \rangle^{-1})$$

where $ZP(\text{Vega})$ is the magnitude of Vega. Under the “CIT” infrared photometry scale, Vega is defined to have $ZP(\text{Vega}) = 0.0$, whereas in the “Arizona” system (e.g., Campins et al. 1985, *AJ*, 90, 896), Vega has $ZP(\text{Vega}) = 0.02$.

5.2.3 Photometric Corrections


Photometric Stability with Time and Temperature

The photometric stability of NICMOS has been monitored throughout the instrument's lifetime using repeated observations of the primary standard stars through a limited set of filters in each camera. During Cycle 7/7N there is evidence for a small drift in the throughput with time, amounting to roughly 2% in this time period. This is to be expected, as the array quantum efficiency is temperature dependent, and the instrument temperature gradually warmed throughout Cycle 7 and 7N.

Since the installation of NCS (Cycles 11 and beyond) there is some evidence for a gradual decline in sensitivity of a few percent over the last six years. This was more surprising, the detector temperatures had been kept stable according to the mounting cup temperature sensors used to stabilize the temperature with the cryo-cooler. However, the mounting cup sensors are not really directly connected to the detectors and by using the temperature-from-bias technique (Section 3.3.1) it has now been shown that the detectors have been cooling down slowly since Cycle 11.

By correlating the count rates of standard stars to the temperature-from-bias measurements we can determine the detector sensitivity dependence on temperature. Figure 5.1 shows an example of the correlation between detector temperature and sensitivity (flux / count rate) for a number of standard stars. This shows that the count rate is increasing for a give flux when the detector temperature increases.


Figure 5.1: Inverse sensitivity as function of temperature

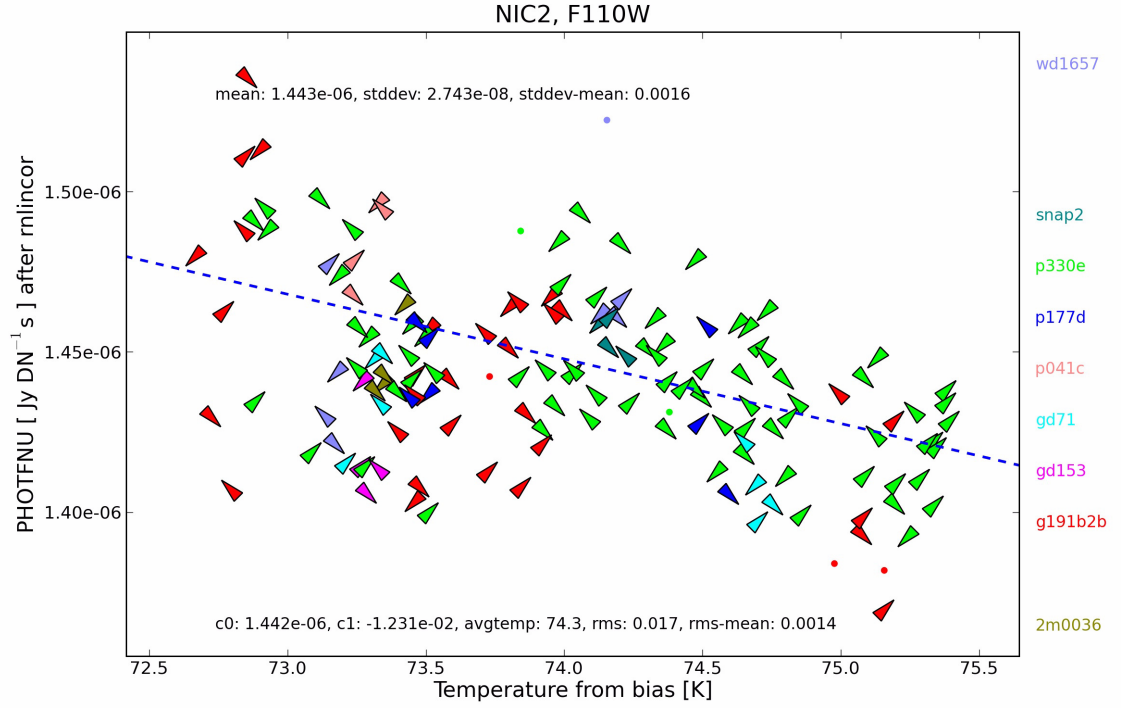

The inverse sensitivity (count rate per unit flux) as function of detector temperature as determined from the bias levels (Section 3.3.1) for Camera 2, F110W observations in the NCS era. Different colors are used to denote different stars as encoded on the right. The point of the triangles indicate the detector quadrant on which the stars were observed. The dashed line indicates the adapted temperature-sensitivity relation.

For Cycle 7/7N there is a wavelength dependence on the slope of this relation as is shown in Figure 5.2. This is most clearly observed for Camera 2, but similar trends are observed for Camera 1 and 3, albeit with much more scatter, and for Cycle 7/7N the same wavelength dependence for all cameras is assumed. For post-NCS data no clear wavelength dependence is found and the same 1.4% per Kelvin sensitivity change is consistent with the data in all filters of all cameras.

Figure 5.2: Temperature dependent sensitivity as function of wavelength

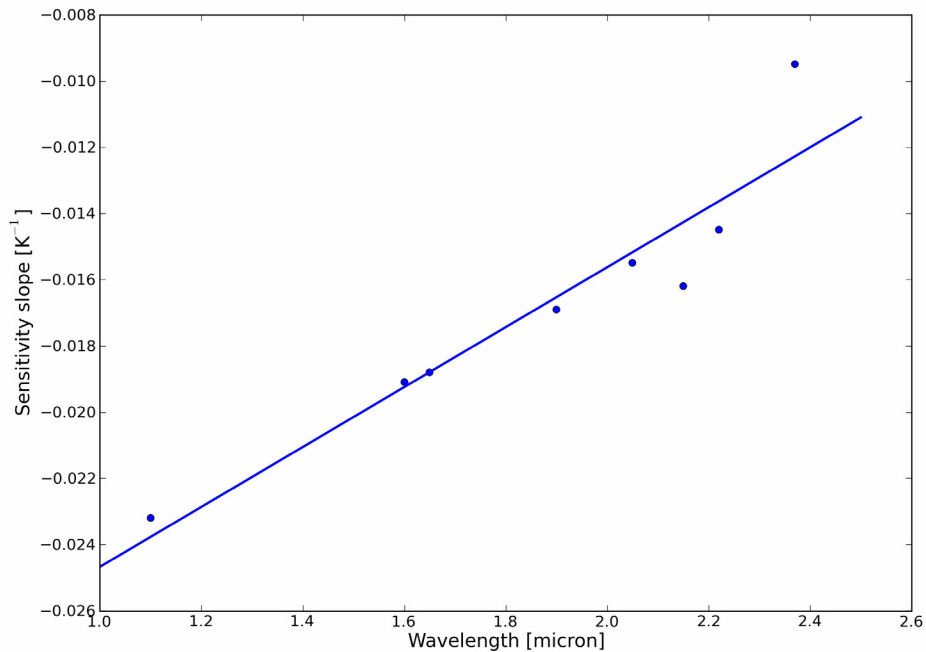

The slope of the temperature-dependent sensitivity correction as function of filter wavelength for Camera 2 observation during Cycle 7/7N (data points) and the adapted relation for all pre-NCS observations (line). There is a clear wavelength dependence for pre-NCS observations, unlike the post-NCS era, where the slope of the correction is about -0.014 for all filters and cameras.

The slopes of the temperature-dependent sensitivity are stored in the PHOTTAB reference file that is also used by calnica to populate the PHOTFNU and PHOTFLAM header keyword items (see Section 5.2.3). When UNITCORR='PERFORM' in the header of an imaging observation and the TFBTEMP header item is within the expected temperature range, calnica will automatically scale the output image to match the PHOTFLAM and PHOTFNU in the header. Scaling the image rather than the modifying the calibration header keywords was chosen to facilitate drizzling of multiple images without further need to scale the images. The scaling factor is stored in the header item ZPSCALE. The scaling by calnica can be switched off by setting PHOTCALC='OMIT'.

Differential Photometry

The photometric values provided in the headers are obtained from measurements of standard stars in the central regions of the detectors. Both high frequency (pixel-to-pixel) and low frequency (large-scale structures) sensitivity variations are corrected using on-orbit flats. On-orbit differential photometry characterization of NICMOS cameras 1 and 2

indicate that residual, large scale deviations amount to $< 2\%$ (rms). Much larger variations are seen for Camera 3, but are due to a different effect, intrapixel sensitivity variations, which we will discuss next.

Intrapixel Sensitivity Variations and Camera 3

As with many other infrared arrays, NICMOS detector sensitivity varies across the area of each physical pixel. It is higher in the center, and lower near the edges. In practical terms, this means that for a source whose flux changes rapidly on a scale comparable with or smaller than that of a pixel, the measured countrate, and therefore the derived flux, will depend on where the center of the source lies with respect to the center of the pixel.

For NICMOS cameras 1 and 2, the PSF is sufficiently well sampled that intrapixel sensitivity variations do not introduce a large (or at least, not a dominant) effect on point source photometry. Camera 3 images, however, are highly undersampled, and the exact position of a point source relative to the pixel grid can introduce large variations in the measured signal. Measurements made using calibration test data, as well as science data with large numbers of dither positions, show that the flux variation can be as large as 30%. The tighter the PSF is, the larger these variations will be. For that reason, “in focus” images taken during the two Cycle 7N refocus campaigns are more subject to the impact of intrapixel sensitivity variations, although the effect is still appreciable for non-campaign data as well. Similarly, stellar images through the shorter wavelength filters (where the telescope diffraction limit is smaller) show a greater variation due to this effect than do longer wavelength data. In addition, the intrapixel sensitivity variations can introduce complications for measuring image centroids, “pulling” the centroid away from pixel corners and edges toward the center of the pixel.

The effects of intrapixel sensitivity variations and possible approaches to correcting NIC3 point source photometry are discussed in two useful references: NICMOS [ISR-99-005](#) (Storrs et al.), available from the STScI web pages, and a paper by Tod Lauer (1999, PASP 107, p.1434). Storrs et al. derive a photometric correction for Camera 3 F110W and F160W stellar images based on a “sharpness ratio,” defined as the ratio of the flux in the peak pixel to that in the integrated PSF. This method is simple to apply and avoids uncertainties due to centroiding errors. Lauer derives a two dimensional pixel response map which can be used to correct photometry if the position of a point source can be measured accurately.

Intrapixel sensitivity variations should have substantially less effect on spatially extended sources. In general, given well dithered data sampling many different sub-pixel positions, the variations due to intrapixel sensitivity should average out, but given the rather large amplitude of the effect for point sources (especially for short wavelength, in-focus NIC3 observations), many dither positions (>10) are probably needed before the

error on the mean count rate is smaller than other sources of photometric uncertainty in NICMOS.



Camera 3 intrapixel sensitivity variations can have a major impact on photometry of point sources. For data taken with fewer than 10 dither positions, this uncertainty may dominate photometric errors unless steps are taken to correct it. We strongly recommend that Camera 3 users concerned with photometry of point sources read the references cited here.

Temporal and Spatial PSF and Focus Variations

The point spread function (PSF) of HST changes with time, and these changes affect photometry using small apertures. The changes can be divided into short-term and long-term effects. The short-term effects are observed on an orbital time scale and are mainly due to thermal breathing of the whole telescope. In addition, the NICMOS PSF varies as a function of position on the array, and this can affect photometry made either with small apertures (by changing the effective aperture correction as a function of position), or using PSF fitting programs such as **daophot** unless there are enough stars in the field for the program to derive a positionally dependent PSF. The focus field variations, however, are relatively small (see [ISR 98-005](#), "NICMOS Focus Field Variations and Focus Centering," Suchkov & Galas 1998; see also NICMOS [ISR 98-018](#) (Suchkov & Krist) for a discussion of the effects of breathing on the PSF modeling). We have used synthetic PSFs from TinyTim (See "Aperture Correction" on page 85.) to determine the positional dependence of the aperture correction as a function of position on NIC2, where the focus field variations are largest. For F110W (the effect should be largest at short wavelengths), the maximum to minimum variation in the aperture correction for photometry measured within a 2 pixel radius is < 2%. The variations are expected to be smaller for the other cameras and for images at longer wavelengths.

The focus field variations after the installation of the NICMOS Cooling System are essentially unchanged compared to Cycle 7 and 7N.

During the pre-NCS era in Cycle 7 and 7N there were long term variations in the NICMOS focus as the cryogen evaporated and the dewar relaxed. The solid nitrogen introduced stress on the instrument, and NICMOS detectors moved along the focus direction as this stress diminished. The change was especially rapid early in Cycle 7. Thereafter the focus remained largely stable for the remainder of the pre-NCS era. The dewar distortion had the greatest effect on the focus of Camera 3, pushing it beyond the range of the Pupil Alignment Mechanism (PAM). For this reason, two special Camera 3 refocus campaigns, each three weeks long,

were undertaken, one from 12 January through 1 February 1998, and the second from 4 June through 28 June 1998. During these periods, the secondary mirror was moved in order to bring Camera 3 into the range where its correct focus could be reached by the PAM. From the post NCS era there has not been any long term effects on the focus for any of the cameras. The focus history of NICMOS can be determined from the focus page of the NICMOS Web site and for further updates please refer to the NICMOS Web page at:

<http://www.stsci.edu/hst/nicmos>

Aperture Correction

It is often difficult to measure the total flux of a point source due to the extended wings of the PSF, diffraction spikes, and scattered light. Such measurements are particularly difficult in crowded fields where the extended wings of sources can overlap with each other. An accurate method of measuring the integrated flux in these situations could consist of several steps:

1. Measure in the image the total counts within a small radius.
2. Simulate the **TinyTim**² PSF for the particular camera-filter combination and position in the detector. **TinyTim** allows the user to simulate PSFs with various focus settings, and users concerned with small focus variations should be careful to set these parameters to the values appropriate for their observations. (This will have the largest effect for NIC3 data taken outside the refocus campaigns.)
3. Use the simulated PSF to measure the fraction of total flux within the photometry aperture.

To obtain the total flux of the source, the countrate then only needs to be multiplied by the `PHOTFNU` or `PHOTFLAM` value and by the inverse of the measured fraction obtained in step three above. The apertures and aperture corrections used to derive the calibration constants in Section 5.2.2 are listed on the [NICMOS photometry Web](#) page.

Empirical PSFs could also be used for the above mentioned method. There have been no special calibration programs to obtain PSF measurements for all camera and filter combinations. A significant amount of PSF data does exist in the archive, however: empirical PSFs for the central regions of the detectors can be obtained from the calibrated images obtained for absolute photometry and photometric monitoring programs.

Out-of-Band Leaks

Many very red targets (e.g., protostars) have been observed with NICMOS at short wavelengths ($\sim 1 \mu\text{m}$). For these sources the flux at

2. **TinyTim** software can be retrieved from the Web at:

<http://www.stsci.edu/software/tinytim/tinytim.html>

$\sim 2.2\text{--}2.5\ \mu\text{m}$ could be orders of magnitude larger than at $\sim 1.0\ \mu\text{m}$ and therefore exceptionally good out-of-band blocking would be required. Pre-launch tests indicated that for very red sources (temperature $\sim 700\ \text{K}$ and lower), some NICMOS filters *might* have significant red leaks. The suspect filters were F090M, F095N, F097N, F108N, F110M, F110W, F113N, F187N and F190N. A limited set of in-flight tests (in calibration programs 7691 and 7904) were made during Cycle 7, observing very red stars to calibrate the possible effects of out-of-band leaks. These data have never been carefully analyzed, but preliminary indications are that actual red leaks are insignificant or non-existent. We nevertheless caution here that this analysis is only preliminary. Users interested in photometry of sources with extreme colors should check the [STScI NICMOS Web](#) pages for updates, or examine the in-flight test photometry of red stars themselves.

Non-Zero Zeroth Read Correction for Bright Sources

The problem of the non-zero zeroth read for bright sources was discussed in Section 3.3.2 (ZSIGCORR) and Section 4.4.2. If significant signal from an object is present in the zeroth read, then this was not properly taken into account in the nonlinearity corrections made for data processed by the OPUS pipeline before 11 November 1997. It is advisable to reprocess the data with the most recent version of the calibration software which includes the ZSIGCORR step to account for this zero read signal correction. When reprocessing such data, **calnica** version 3.3 or greater will automatically apply this step to all MULTIACCUM mode observations if both ZOFFCORR and NLINCORR are also being performed. All data retrieved from the Archive via OTFR after 26 September 2001 are automatically processed with this step.

Magnitudes and Photometric Systems Transformations

As was previously mentioned, NICMOS data are calibrated in units of Jy or Jy arcsec^{-2} for flux densities and surface brightnesses, respectively. The filter bandpasses do not exactly match those of ground-based JHK filters, and therefore if you wish to derive standard JHK magnitudes from NICMOS data, then it will be necessary to apply a color term correction. The recommended NICMOS JHK-analog system is obtained using the F110W, F160W and F222M filters, although the F110W filter especially is quite different from the standard J bandpass (specifically, it is much broader and bluer). Synthetic color terms can be computed using **synphot**, given real or model spectra for an astronomical source and the NICMOS and ground-based filter bandpasses (see, for example, Holtzman et al. 1995, PASP 107, 1065, where a similar procedure was used to derive color terms for WFPC2 photometry).

Also, as part of the absolute photometry program, we observed a few blue stars (white dwarfs), intermediate color stars (solar analogs), and very red stars covering a large range in color (Table 5.1). The calibrated data are available from the archive for users who wish to derive their own color terms to transform their *HST* fluxes into any ground-based system. The ground-based photometry given in the table below is based on preliminary and incomplete measurements, and will be updated when the final NICMOS photometric calibrations are completed.

Table 5.1: List of Stars for Photometric Transformations

Name	H	J-H	H-K	Status	Program IDs
G191-B2B	12.6	-0.10	-0.14	Primary standard (white dwarf).	7691, 7816, 8986, 9997, 9998, 10381, 10725, 11060
P330E	11.6	0.28	0.07	Primary standard (solar analog).	7691, 7816, 8986, 9997, 9998, 10381, 10725, 11060
OPH-S1	7.3	1.53	0.94	Primary standard (red standard).	7049, 7691
P177D	12.0	0.28	0.06	Secondary standard (solar analog).	7904, 7816, 7902, 7904, 9997, 9998, 11061
CSKD-12	9.5	2.08	0.89	Secondary standard (red standard).	7904, 7816
BRI0021	11.1	0.75	0.52	Secondary standard (red standard).	7904, 7816, 10454

5.2.4 Absolute Photometry for Emission Line Filters

The narrow band filters in NICMOS are intended primarily for observations of emission or absorption lines in sources. Because the photometric conversion factors $PHOTFNU$ and $PHOTFLAM$ for all NICMOS filters are obtained from continuum observations of emission-line free standard stars, the flux in $\text{erg sec}^{-1} \text{cm}^{-2}$ of an emission line is given by the expression:

$$Flux_{line} = 1.054 \times FWHM \times PHOTFLAM \times CR$$

where FWHM is the full width half maximum of the equivalent gaussian filter to the narrow-band filter used (see [Appendix A of the NICMOS Instrument Handbook](#), and we have assumed that the continuum has been already subtracted from the total flux in the filter and that the line is centered in the filter. If the emission line is not at the central wavelength of the filter, the line flux will need correction for the filter transmission curve.

To estimate the variation in the absolute flux due to the positioning and width of the emission line in the filter bandpass, the **synphot** task **calcphot** can be used as shown below. See the *Synphot User's Guide* for additional help.

Figure 5.3: Estimating Absolute Flux Variation

```
sy> epar calcphot
obsmode = nicmos,3,f212n,dn Instrument observation mode
spectrum= gauss(21200,40)*unit(1E-13,flam) Synthetic spectrum to calculate
form = counts Form for output data
(func = effstim) Function of output data
(vzero = ) List of values for variable zero
(output = none) Output table name
(append = no) Append to existing table?
(wavetab= ) Wavelength table name
(result = 0.) Result of synphot calculation for form
(refdata= ) Reference data
(mode = a)

sy> epar calcphot
obsmode = nicmos,3,f212n,dn Instrument observation mode
spectrum= gauss(21280,40)*unit(1E-13,flam) Synthetic spectrum to calculate
form = counts Form for output data
(func = effstim) Function of output data
(vzero = ) List of values for variable zero
(output = none) Output table name
(append = no) Append to existing table?
(wavetab= ) Wavelength table name
(result = 0.) Result of synphot calculation for form
(refdata= ) Reference data
(mode = a)
```

The examples in Figure 5.3 compute the countrate in the NIC3 F212N filter for a H₂ (2.12 micron) emission line having a gaussian profile of 40 Angstroms and a peak flux of $1.0 \times 10^{-13} \text{ erg sec}^{-1} \text{ cm}^{-2} \text{ A}^{-1}$. The integrated flux will then be $4.2 \times 10^{-12} \text{ erg sec}^{-1} \text{ cm}^{-2}$. In the first example the H₂ emission line is at zero redshift and centered on the filter while in the second example the line is redshifted by 80 Angstroms. If the emission line is centered on the filter, the H₂ flux will produce 7421.1 DN sec⁻¹ while the countrate will be ~90% of this value (i.e., 6662.3 DN sec⁻¹) for the redshifted emission line. The expression for the Flux_{line} above can be directly applied to the first case, while a correction factor $1.11 = (7421.1/6662.2)$ is needed in the second case.

5.2.5 Absolute Spectrophotometry with NICMOS Grisms

The accuracy of the absolute spectrophotometry with NICMOS grisms depends on three limiting factors:

- Accuracy of the spectral energy distribution of the standard stars used to obtain the inverse sensitivity curve.
- Quality of the flat-fielding and background subtraction of the calibration observations.
- Quality of the flat-fielding and background subtraction of the science observation itself.

The major source of uncertainty in the absolute spectrophotometry of a given source comes from the variability and structure of the background. Every pixel on the NIC3 array will receive background radiation over the entire spectral bandpass of the particular grism, while the source spectrum will be dispersed. The accuracy of the background subtraction is limited by our knowledge of the spectral response of each pixel, which is somewhat different from pixel to pixel. Extracted spectra will have to be corrected for the spectral response of each pixel. The accuracy of this correction is again limited by our knowledge of the detector response.

Remember that the spectra are not aligned with the X axis of the detector, and therefore move from one row to the next. This makes grism spectra especially sensitive to the intrapixel sensitivity variation. The **NICMOSlook** and **aXe** software (see Section 5.7) have a capability built in to correct for this variation which depends critically on the placement of the spectrum. The software handbook describes an iterative procedure to determine the best correction for this problem.

The absolute flux calibration of the spectral energy distribution of the standard stars in the 0.8 to 2.5 μm wavelength range is known to 2–5%. Grism data reduction and calibration are discussed in more detail in Section 5.7.

5.3 Astrometry, Pixel scales, and Geometric Distortion

Accurately transforming pixel positions in NICMOS images to relative or absolute astronomical coordinates involves several considerations. Here we consider each of these in turn. For the latest information regarding these issues, consult the STScI NICMOS plate scale Web pages at: <http://hst.stsci.edu/nicmos/performance/platescale>.

5.3.1 Pixel Scales

With the installation of NCS, the plate scale of NICMOS has become very stable. The NICMOS arrays are slightly tilted relative to the focal plane, and therefore the NICMOS pixel scales along the X and Y axes of each camera are slightly different, i.e., projected on the sky, the pixels are actually slightly rectangular, not square. The X and Y plate scales at the central pixel of the arrays are listed in Table 5.2 and were determined from SMOV3b data as described in more detail in Section 5.3.2. The differences in X and Y pixel scale are small: the X/Y scale ratios S_X/S_Y are approximately 1.0030, 1.0076, and 1.0032 for cameras 1, 2 and 3, respectively, in the sense that the X scale in arcseconds per pixel is larger than the Y scale in each case. It amounts to 1 to 2 pixels “extra width” in the X direction relative to Y over the field of view of the cameras, and for

precision astrometry or when registering NICMOS images to data taken with other instruments such as WFPC2, it may be important to take the effect into account. This can easily be done when drizzling NICMOS images using coefficient matrices as described in Sections 5.3.2 and Section 5.3.3 below.

During Cycle 7, the distortion of the NICMOS dewar due to the cryogen expansion affected the optical path, pushing the cold well and cameras closer to the field divider assembly and cold mask. This caused the effective focal length, and hence the pixel scale, to change somewhat as a function of time during Cycle 7. The changes were most rapid during the orbital verification period and approximately the first 100 days of instrument operations, then slowed, with only small variation thereafter. The pixel scale was monitored regularly throughout Cycle 7. A tabular and graphical record of these measurements for all three cameras can be found on the STScI NICMOS Web pages at:

<http://hst.stsci.edu/nicmos/performance/platescale>.

This source should always be consulted before transforming pixel coordinates of Cycle 7 images to arcseconds.

Table 5.2: NICMOS Plate Scales at Detector Center (i.e. pixel 128, 128)

	NIC1 ("/pixel)	NIC2 ("/pixel)	NIC3 ("/pixel)
X	0.043142	0.075948	0.203127
Y	0.043014	0.075355	0.202600

5.3.2 Geometric Distortion

The distortion corrections for the NICMOS cameras are small, but for precision astrometry or when registering and coadding images (especially taken with a wide dither pattern, or when assembling mosaics covering a large field) it should be taken into account. The geometric distortion was measured using dithered observations of the astrometric field NGC1850 through all three cameras. The data analysis and results for Cycle 7 are described in detail in an instrument science report (ISR) by Cox et al. 1997 (ISR OSG-CAL-97-07). The same technique was used to determine the distortions after NCS installation, using data obtained during SMOV3b. An ISR describing analysis of these data is forthcoming, but results are listed in Table 5.3, on the [NICMOS pixel scale Web page](#), and are incorporated in the latest drizzle coefficient files (see Section 5.3.3).

The maximum total positional deviations (in pixels), assuming zero distortion at field center, are approximately 0.9, 0.25, and 0.75 pixels for Cameras 1, 2 and 3, respectively. Cox et al. found that quadratic relations

were adequate for describing the distortion given the accuracy of the observational measurements. Given a pixel position (x,y) , we define new coordinates (x',y') relative to the array center, here chosen to be at pixel 128,128:

$$x' = x - 128,$$

$$y' = y - 128.$$

The positions corrected for distortion, (x_c', y_c') , are then given by

$$x_c' = a_{10} x' + a_{11} y' + a_{20} x'^2 + a_{21} x' y' + a_{22} y'^2$$

$$y_c' = b_{10} x' + b_{11} y' + b_{20} x'^2 + b_{21} x' y' + b_{22} y'^2$$

where the origin of the (x_c', y_c') coordinate system is chosen to be coincident with that of (x', y') , i.e. pixel (128,128) of the array. As defined by Cox et al., the distortion corrections explicitly do not account for the X and Y scale difference described above, and therefore a_{10} and b_{11} are fixed at 1. The actual plate scales at pixel (128, 128) are listed in Table 5.2 for data taken after NCS installation or can be obtained from the Web as described in Section 5.3.1. Also, a_{11} (the linear dependence of x on y) is held at 0, although b_{10} is derived in the fit. This fixes the y axis orientation, but allows for departures from orthogonality. The fitted coefficients for the three cameras are given in Table 5.3.

Table 5.3: NICMOS Geometric Distortion Coefficients

	NIC 1		NIC 2		NIC3 (y>15)	
Coefficient	value	±	value	±	value	± ±
a ₁₀	1.0	3.33e-5	1.0	4.17e-5	1.0	4.34e-5
a ₂₀	-6.017980e-6	1.48e-7	5.457250e-6	2.34e-7	6.200932e-6	8.23e-7
a ₂₁	1.321113e-8	1.11e-9	2.349997e-9	2.25e-10	-3.575648e-8	2.17e-9
a ₂₂	-2.281896e-5	8.01e-9	1.366225e-6	2.73e-8	-9.335416e-6	3.30e-7
b ₁₀	-1.568197e-3	3.33e-5	1.455222e-3	4.17e-5	-2.238978e-3	4.34e-5
b ₁₁	1.0	1.26e-5	1.0	6.28e-6	1.0	2.55e-5
b ₂₀	-5.854990e-65	1.48e-7	1.427241e-6	2.34e-7	-1.791625e-5	8.23e-7
b ₂₁	1.534969e-7	1.11e-9	4.777928e-8	2.25e-10	-2.555493e-9	2.17e-9
b ₂₂	2.406571e-5	8.01e-9	1.168855e-6	2.73e-8	1.857704e-7	3.30e-7

After applying this distortion correction, remember to add 128 to each of the x_c' and y_c' values to transform the origin back to pixel position (128,128).

Also remember that the above solution does *not* correct the X/Y scale differences described above. The preferred way to do this would be to multiply all the a coefficients in the expression above by the square root of the pixel scale ratio, $\sqrt{(S_X/S_Y)}$, and the b coefficients by the reciprocal

value, $\sqrt{(S_Y/S_X)}$, using the scale ratios given above. This will correct all pixels to square geometry, preserving the area of a pixel located at array center. This is the approach used in the distortion coefficients used by the **drizzle** algorithm (see Section 5.3.3).

Cox et al. also solve for the detector y axis orientation relative to the telescope V3 axis. The beta angles (Bx and By), shown in Table 5.4, indicate the angle of the +x and +y axes from the telescope +V3 through +V2 in degrees (see Fig 6.1 in the NICMOS Instrument Handbook).

Table 5.4: Beta Angles for all Three NICMOS Cameras

	Bx (degrees)	By (degrees)
NIC1	225.71	315.80
NIC2	224.79	314.71
NIC3	225.06	315.19

5.3.3 Drizzling

One way to apply the geometric distortion correction when combining dithered NICMOS images is to use the **drizzle** software, which is incorporated into the package **stsdas.analysis.dither**. This software was written to allow geometric distortion corrections to be applied during drizzling. In order to do so, it is necessary to specify a coefficient file with the parameter `drizzle.coeffs`. Geometric distortion coefficient files in a format suitable for use with **drizzle** are available from the [STScI NICMOS Web](#) pages and are also provided with the **stsdas.analysis.dither** package. In these, the coefficients from Cox et al. have been multiplied by the square root of the pixel scale ratio so that the output images will have square pixels with uniform X and Y scales, as described above. The absolute pixel scale (arcseconds per pixel) is not set by the drizzling procedure, and should be determined by using `drizzleinfo` or by consulting the [NICMOS pixel scale Web](#) page, as explained above. The appropriate value to use with the drizzled images is the geometric mean of the X and Y scales specified by the Web pages, i.e. $\sqrt{S_X \times S_Y}$.

The latest version of **MultiDrizzle**, available in **stsdas.analysis.dither** now fully supports NICMOS observation and is to date the easiest way to apply geometric correction to NICMOS observations. **MultiDrizzle** applies the same corrections described above when using **drizzle**. However, the distortion coefficient files for all three NICMOS detector are now available as part of the routine NICMOS calibration files and these will be used automatically by **MultiDrizzle**. Users should refer to the NICMOS example of the **MultiDrizzle** Cookbook for a much more detailed example of how using **MultiDrizzle** with NICMOS data.

5.3.4 Absolute Astrometry

As with all *HST* instruments, determining the absolute astrometry in NICMOS images to good accuracy requires precise astrometry from some external source for at least one object within the field of view. The absolute pointing reference given by world coordinate system (WCS) information encoded in NICMOS image headers is derived from the *HST* Guide Star Catalog (GSC) positions for the stars used to guide the observations. Although the GSC positions, and hence the WCS astrometry, are generally good, deviations by as much as 2 arcseconds from an absolute celestial reference frame (e.g., FK5) are not uncommon. The WCS information provided with NICMOS images does account (at least to first order) for the nominal pixel scale, camera orientation, and even the X and Y pixel scale differences of the cameras. It does not, however, include any higher order corrections for geometric distortion. Therefore relative positions measured using the WCS (e.g., with the **IRAF** tasks **imexam** or **rimcur**) are fairly accurate, even if the absolute pointing reference may not be exact.

Finally, it is important to note that precise astrometry with NIC3 can be complicated by three effects. First, for data taken outside the January or June 1998 refocus campaigns, focus effects may affect the geometry of the focal plane. Second, data taken prior to January 1998 was usually vignetted (see Section 4.7.4), which can also distort the geometry. Finally, intrapixel sensitivity variations (see Section 5.2, and NICMOS [ISR-99-005](#), Storrs et al.) can affect centroiding for undersampled point source images.

5.4 PSF Subtraction

Accurate PSF subtraction is a prime concern for an observer wishing to study faint features around bright objects. Typical situations are: a host galaxy harboring a bright quasar; circumstellar nebulosity around a bright star; faint companions of a bright star, etc. PSF subtraction for NICMOS data can be very effective, especially for images from cameras 1 and 2, thanks to a few important features of this instrument:


- Cameras 1 and 2 provide images which are diffraction limited, and well sampled (see Figure 5.4 and Figure 5.5).
- The MULTIACCUM mode automatically provides sub-exposures with different exposure times, and **calnica** processing will use only unsaturated data values when constructing the calibrated image.
- For a saturated bright central point source, there is no blooming along the detector array columns as there is with a CCD.

One way to get a high quality PSF for subtraction is to measure an isolated bright unsaturated star in the same image or to construct a


composite PSF using good stars in the image. This can be accomplished using the **IRAF digiphot** package as described in *A User's Guide to Stellar CCD photometry with IRAF*³. A PSF obtained from the same image ensures that effects of telescope focus and pointing jitter on the image quality are properly taken into account. In particular, this approach will take care of the *breathing* effect: variations of focus position due to thermally induced mechanical displacements in the *HST* optical path. One disadvantage of this method, however, is that it is difficult to account for positional variations in the PSF over the field of view of the NICMOS cameras (see discussion in Section 5.2.3, and also in Suchkov & Galas 1998, NICMOS [ISR 98-005](#)). Although these variations do not have a large affect on NICMOS aperture photometry, they can be large enough to cause problems for PSF matching and subtraction. If no suitable star can be found in the image, one can resort to a synthetic PSF computed using **TinyTim**.

Figure 5.4: NIC1 Image with PSF Radial Profile

Image of Star Taken with NIC1 F165M

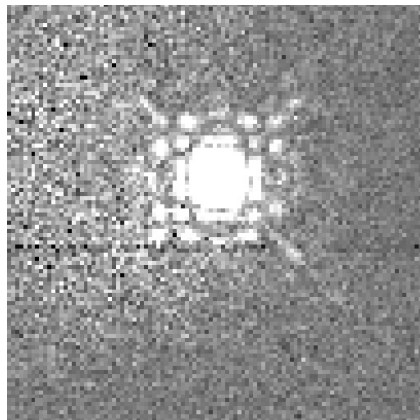


PSF Radial Profile

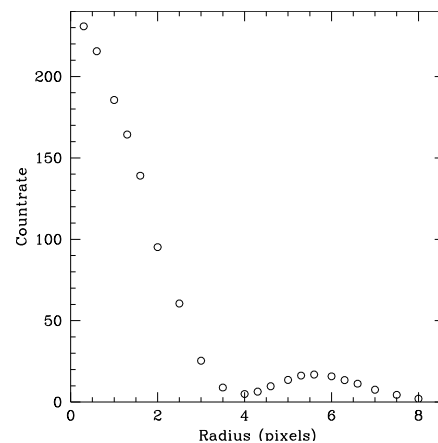


3. This and other relevant IRAF documents can be obtained from the IRAF Web site at: <http://iraf.noao.edu/>.

Figure 5.5: NIC2 Image with Radial Profile

Image of Star Taken with NIC2 F237M

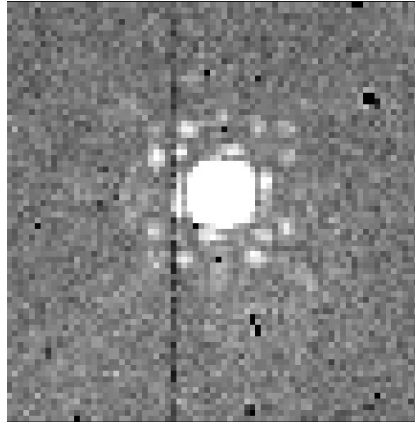

PSF Radial Profile

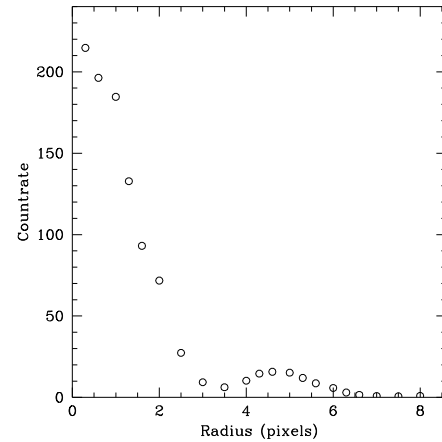

5.4.1 Impact of Instrumental Effects on PSF Subtraction

There are a number of factors which affect the NICMOS PSF and thus can impact the results of image analysis relying on PSF subtraction. The factors are: focus variations due to OTA breathing, cold mask irregular motion (“wiggling”) on an orbital time scale, PSF color dependence.

The limits to the accuracy of PSF subtraction imposed by these factors have been assessed using model PSFs generated by **TinyTim** software and **synphot** generated blackbody spectra. The results for Camera 2 are given in Table 5.5 below. The mean and standard deviation of the PSF subtraction residuals are given a percentage of the nominal PSF pixel values. The standard deviation can be interpreted as the average relative spatial noise expressed as a percent of the PSF pixel value at any given distance from the PSF center. The mean represents a systemic component in the PSF residuals.


Table 5.5: Effect of focus variation, cold mask wiggling, and PSF color dependence on PSF subtraction.

effect of:	mean sigma F187W	mean sigma F187N	mean sigma F160W	mean sigma F187N	mean sigma F110W	mean sigma F187W
focus variation	0.62% 6.81%	1.86% 17.29%				
cold mask wiggling			0.10% 14.38%	3.15% 37.67%		
color dependence (8000K-3000K)					23.50% 8.91%	0.58% 1.57%
color dependence (8000K-6000K)					-1.52% 1.32%	
color dependence (6000K-3000K)					25.31% 7.32%	

The effects of both cold mask wiggling and focus breathing introduce errors in a PSF-subtracted image, well above 20% of the PSF signal in a narrow band filter, with a spatial scale of a few pixels. The main effect of PSF color dependence is adding a systemic component to the PSF subtracted image. The effect is quite large if the color of the PSF used for subtraction is very different from the image PSF color. It is pronounced in blue, wide filters, like F110W, while in filters like F187W or redder/narrower it is essentially negligible. The best way to cope with this effect is to use PSFs with colors well matched to the sources.


PSF subtraction with NICMOS Camera 3 is extremely difficult due to the large pixel scale which severely undersamples the point spread function, and because of the strong intrapixel sensitivity variations (see Section 5.2.3) which affect the structure of point source images.

Figure 5.6: Effect of cold mask wiggling on PSF subtraction in broad band and narrow band filters.

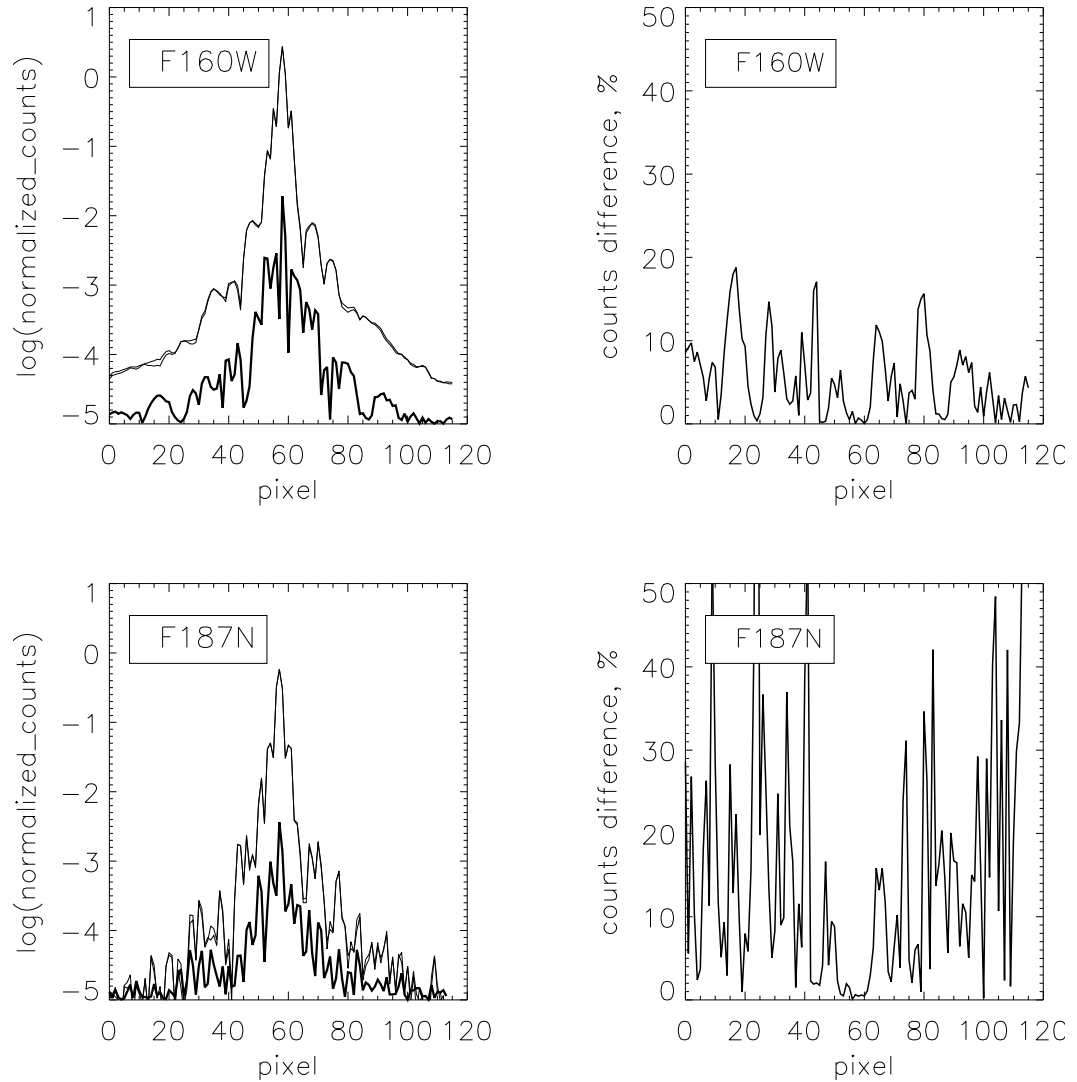


Left panels: normalized counts (log scale) in the central column of the two **Tiny-Tim** PSFs with 0.005 difference of the cold mask offset (thin lines). The thick line is the difference between the two. Right panels: absolute value of counts difference as a percent of the counts for the PSF at the “nominal” cold mask offset.

Figure 5.7: Illustration of PSF color dependence in different filters.

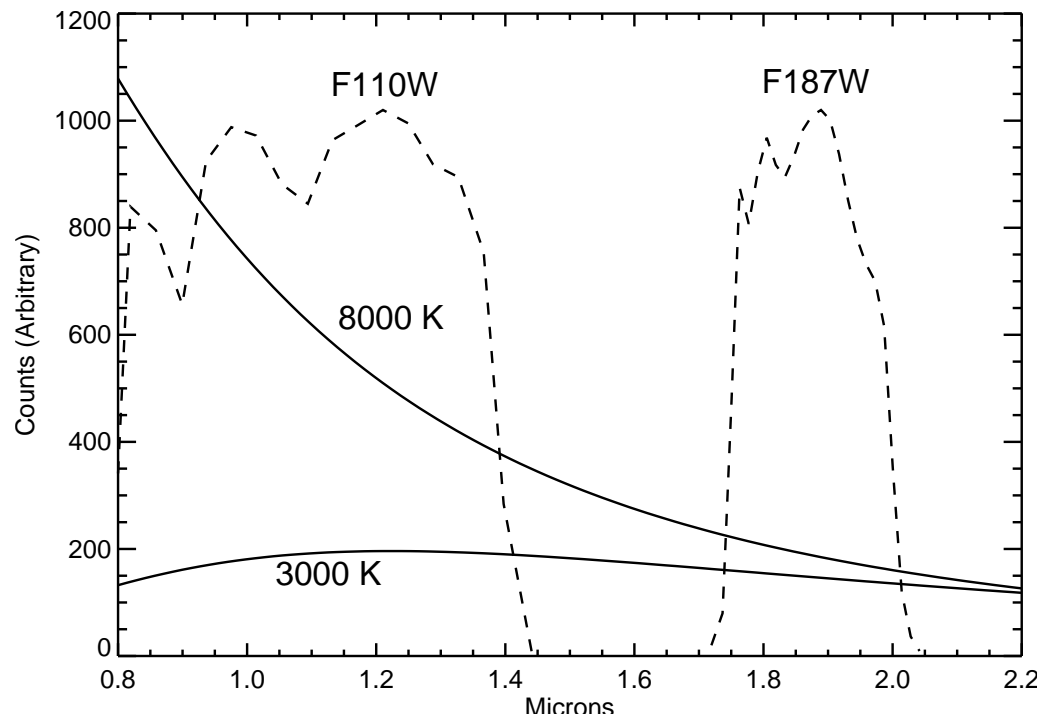

In F110W, the 8000 K blackbody spectrum has a very different slope from that of the 3000 K blackbody. Therefore the PSF resulting from images of point sources with these temperatures will be very different from one another. The F187W filter, however, samples the Rayleigh-Jeans regime for both temperatures, resulting in spectra with about the same slope, so the difference between the 8000 K PSF and 3000 K PSF will be very small.

Figure 5.8: Effect of PSF color dependence on PSF subtraction in different filters.

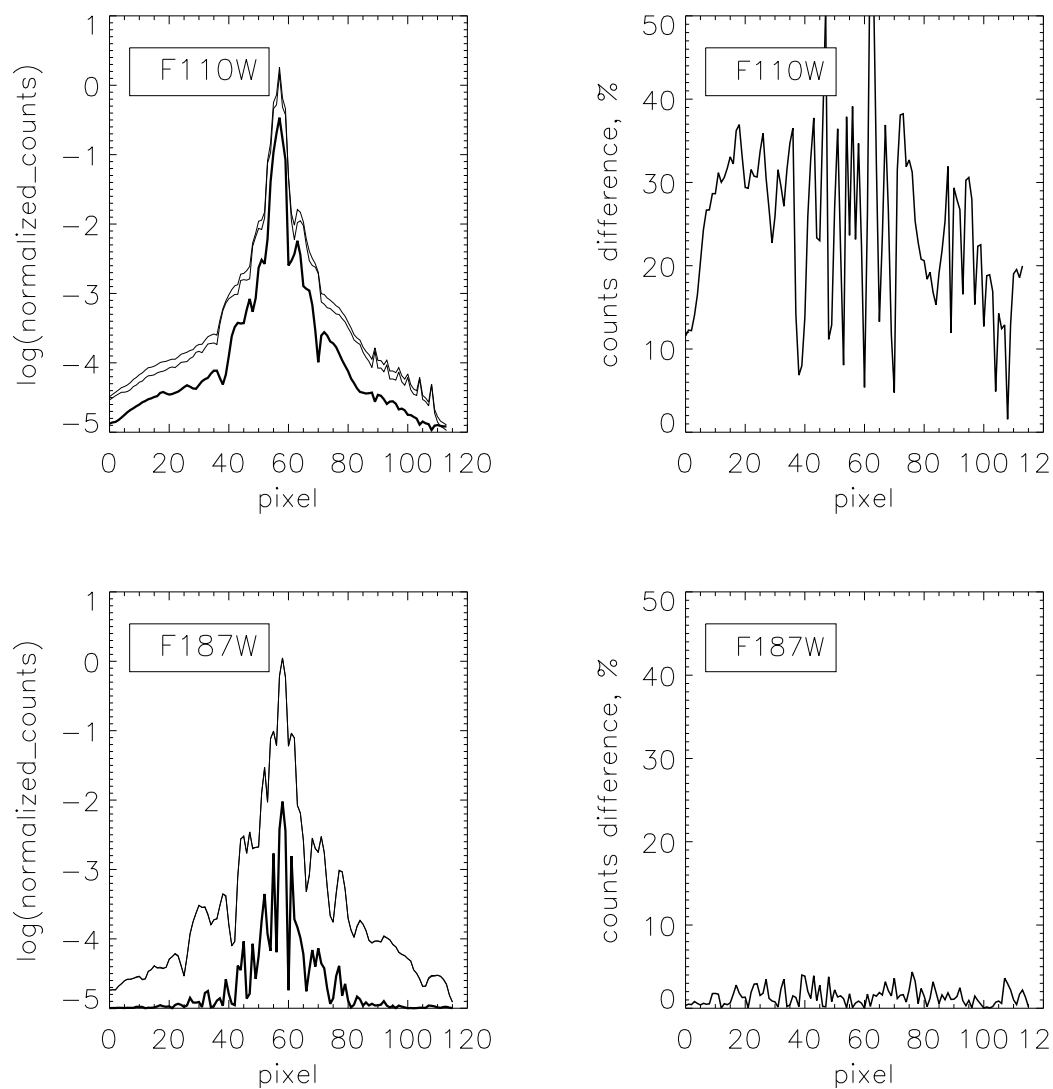

Left panels: normalized counts (log scale) in the central column of TinyTim 8000 K and 3000 K blackbody PSFs (thin lines). The thick line is the difference between the two. Right panels: absolute value of counts difference as a percent of counts for the 8000 K PSF.

5.5 Coronagraphic Reductions

5.5.1 Data Products and File Structures

NICMOS coronagraphic observations consist of an acquisition image and science observations. The acquisition could be an onboard acquisition performed by the NICMOS flight software (FSW) during the same visit as the science observations. Or, a real time acquisition may have been performed by sending the acquisition image(s) to the ground for analysis by the Observation Support System (OSS) and Post-Observation Data Processing System (PODPS) Unified System (OPUS) personnel during the first visit of a two visit observation set. The accompanying science observations would have been obtained during the second visit. The ACCUM, BRIGHTOBJ, and MULTIACCUM observing modes have all been used for acquisitions and for the science observations. Each type of data requires different calibration steps and dark reference files.

5.5.2 Coronagraphic Acquisitions

Coronagraphic imaging requires an acquisition sequence at the beginning of the visit to center the target in the coronagraphic hole. The size of the coronagraphic hole is smaller than typical *HST* blind-pointing errors. The procedure for a coronagraphic acquisition is to first image the target in Camera 2 using blind-pointing, then use either an onboard (Mode-2 Acquisition), Reuse Target Offset (RTO), or a fully interactive acquisition method. A telescope slew is calculated and commanded to move the position of the hole over the image of the target.

The target is positioned on the NIC2-CORON aperture, which has the aperture fiducial point at the image position of the coronagraphic hole on the detector. The science exposures are then specified using any of the NICMOS observing modes and any of the NIC2 filters.

During the Second Servicing Mission (SM2) Orbital Verification (SMOV) commissioning of the coronagraphic observing mode, it was determined that decentering a point source from the center of the coronagraphic hole by a small amount ($x=-0.75$, $y=-0.25$ pixels) reduced the scattered light background intensity. This offset was implemented in the NICMOS ACQ flight software for use in Cycle 7 and 7N science observations. During recommissioning following SM3B, the low scatter point was determined to be at pixel location $x=-0.75$, $y=-0.05$ from the hole center. This offset was implemented for Cycle 12 and later science observations.

The various modes of NICMOS coronagraphic acquisition and the processing required to analyze the resulting data are described in detail in a

series of Instrument Science Reports (ISRs) by Schultz et al., which are available from the STScI Web pages. Users analyzing coronagraphic data, or planning future coronagraphic observations, should carefully read NICMOS [ISR-97-031](#), [ISR-98-012](#), [ISR-98-019](#), and [ISR-99-006](#). A discussion of the coronagraphic performance in Two-Gyro mode is presented in NICMOS [ISR 2005-001](#). Some important highlights for understanding and reducing coronagraphic data are summarized in this Handbook, but the reader should consult the ISRs for more detailed discussions.

Onboard Acquisition

In Mode-2 acquisition (see NICMOS [ISR-98-012](#), Schultz et al.), the onboard NICMOS flight software (FSW) will locate the position of the coronagraphic hole and target. It will use this information to calculate an offset to slew the telescope to position the image of the hole over the position of the target. The location of the coronagraphic hole is determined from pointed flat-field observations. Two short ACCUM F160W filter exposures (7.514 seconds each) with calibration Lamp 1 on (flat field) and two identical exposures with the lamp off (background) are obtained before the acquisition images. The telescope is NOT slewed to move the target out of the FOV during the lamp-on and background observations. The image of the target will be superimposed on these images.

The flight software combines the two background and two flat-field images, subtracts the background image from the flat-field image, and determines the position of the hole. These temporary difference images are not saved. The location of the hole is temporarily stored onboard, but it is not included in the science telemetry. The target position and the slew are stored within the embedded engineering attached to the data set. This information is extracted from the engineering telemetry and written to the science header of the observation following the ACQ, `ipppss00t_raw.fits`. The two flat-field images are written to image `ipppssoot_rwf.fits` and the two background images are written to image `ipppssoot_rwb.fits`.

An error in the Flight Software code prior to June 28, 1998 resulted in errors in the determination of the image position of the coronagraphic hole. Usually, this error was at the sub-pixel level and occasionally was off by a pixel. The decentered imaging affected the coronagraphic performance. It was corrected after this date.

The acquisition aperture is a square area on the detector, a 128 x 128 pixel aperture (center at 157, 128) of size 9.6 x 9.6 arcseconds. Two ACCUM images of equal exposure are obtained, and are saved together in

a single fits file `ipppssoot_raw.fits`. A summary of the files produced in an ACQ data set is presented in Table 5.6.

Table 5.6: NICMOS ACQ Data Image Extensions

Extension	Image Contents
<code>ipppssoot_raw</code>	Raw science data file
<code>ipppssoot_rwb</code>	Raw background data file
<code>ipppssoot_rwf</code>	Raw flat-field data file
<code>ipppssoot_spt</code>	Target SHP and UDL information
<code>ipppssoot_spb</code>	Background SHP and UDL information
<code>ipppssoot_spf</code>	flat-field SHP and UDL information
<code>ipppssoot_cal</code>	Calibrated science data file
<code>ipppssoot_clb</code>	Calibrated background data file
<code>ipppssoot_clf</code>	Calibrated flat-field data file
<code>ipppssoot_trl</code>	OPUS processing trailer file
<code>ipppssoot_pdq</code>	OPUS Processing Data Quality file (discontinued May 9, 2002)



During Cycle 7 and 7N, the `exptime` keyword for NICMOS ACQs was incorrectly populated. A correction was installed in OPUS 9.4, on October 19, 1998.

Reuse Target Offset (RTO) and Interactive Acquisitions

A variation of the Reuse Target Offset (RTO) capability is sometimes used to acquire and position bright targets into the coronagraphic hole. This is known as Mode-1 acquisition (see Schultz et al., NICMOS [ISR-98-019](#)). Any target that would saturate the detector in the shortest possible Mode-2 ACQ ACCUM exposure time, 0.228 seconds, was considered to be a bright target. The following discussion describes the necessary steps for a Mode-1 Reuse Target Offset (RTO) acquisition. The RTO acquisitions are performed during the first visit and the science observations are obtained in a following second visit.

Images of the target and coronagraphic hole are obtained a few orbits in advance of the coronagraphic observations, and sent to the ground for analysis (RT ANALYSIS). The same roll of the spacecraft is used for both the acquisition and science visits. Usually, the same dominant and subdominant guide stars are used for both the acquisition and science

observations. However, in a few instances, this is not the case; after the slew is performed, the target is found outside of the hole, either on the edge of the hole or far from the hole. The coronagraphic observer as well as future Archive users are advised to check the `ipppssoot_spt.fits` files for the guide stars used for the ACQ and science observations (keywords `DGESTAR`, `SGESTAR`).

The background and flat-field observations are usually offset as much as 18-25 arcseconds from the target position to avoid the diffraction spike from the image of an overexposed target crossing the coronagraphic hole and introducing errors in the measured position of the coronagraphic hole. OPUS staff assist the PI in identifying the target, centroiding, and determining offsets.



Information that an RTO has executed is currently stored in an operational database and not available to GO's or archival users.

5.5.3 Positions of the Hole and Target

The location of the target and the slew are saved in the embedded engineering data attached to the science observations. These values are recovered from the embedded engineering data and written to keywords (`NXCENT`, `NYCENT`, `NOFFSETX`, `NOFFSETY`) in the RAW file. The first observation following the NICMOS ACQ will contain the updated values. The target location and slew values of the most recent target acquisition will be reflected in following observations until the next acquisition executes, or until the values are re-initialized to zero. These values are not initialized during normal operation of NICMOS.

As presented, the keyword values are scaled ENGINEERING units, and not in pixels or arcseconds. They must be converted from ENGINEERING units to DETECTOR and IMAGE coordinates.⁴

Target Position in Detector Coordinates

The target position coordinates (`NXCENT`, `NYCENT`, `NOFFSETX`, `NOFFSETY`) can be converted into DETECTOR coordinates by dividing by 256. However, the slew values are written in 2's complement. A value less than 32757 is positive, while a value larger than 32757 is negative. Slew values need to be divided by 128 during the conversion into DETECTOR coordinates. For example, the following target and slew values were obtained from a RAW file and converted to DETECTOR coordinates.

4. NICMOS [ISR 98-012](#)

```

> hedit n4q832nrq_raw.fits[1] NXCENT,NYCEN,NOFFSETX,\
>>> NOFFSETY .
n4q832nrq_raw.fits[1],NXCENT = 31418
n4q832nrq_raw.fits[1],NYCENT = 20655
n4q832nrq_raw.fits[1],NOFFSETX = 10101
n4q832nrq_raw.fits[1],NOFFSETY = 52259

NXCENT = 31418.0 / 256.0 = 122.726
NYCENT = 20655.0 / 256.0 = 80.683
NOFFSETX = 10101.0 / 128.0 = 78.914
NOFFSETY = (52259.0 - 65535.0) / 128.0 = -103.718

```

The position of the coronagraphic hole can then be inferred by subtracting the offset slew and the coronagraphic hole offset from the position of the target.

```

NXHOLE = 122.726 - 78.914 - 0.25 = 43.562
NYHOLE = 80.683 + 103.718 - 0.75 = 183.651

```



*A fix was included in OPUS 9.2, which was installed July 16, 1998. The slew and target position keywords **NXCEN**, **NYCEN**, **NOFFSTX**, and **NOFFSTY** were added to the SPT file. These keyword values are in detector coordinates.*

```

NXHOLE = NXCEN-NOFFSTX
NYHOLE = NYCEN-NOFFSTY

```

The IMAGE coordinate system for NICMOS Cameras 1, 2, 3 have been defined such that the origin will be in the lower left hand corner when displayed, while DETECTOR coordinates are defined by the readout directions for each camera. Any NICMOS camera image, when displayed using the **IRAF display** command, will be displayed relative to the *HST* field of view as depicted in the NICMOS Instrument Handbook. The conversion from DETECTOR coordinates to IMAGE coordinates is performed during OPUS pipeline processing. For Camera 2, the OPUS +x direction is

detector -y direction, and correspondingly, the OPUS +y direction is detector -x direction. Care must be exercised when converting from one coordinate system to the other.

$$\begin{aligned}\text{NXHOLE}(\text{IRAF}) &= 256.5 - 183.651 = 72.849 \\ \text{NYHOLE}(\text{IRAF}) &= 256.5 - 43.562 = 212.938\end{aligned}$$

Measuring the Hole Position

The coronagraphic hole location can be determined from off-line processed ACQ images and should be very close to the inferred location of the hole determined by subtracting the FSW slew from the FSW target position. However, the hole pattern is not symmetric about the low scatter point (pixel with least counts) of the OPUS pipeline processed coronagraphic hole image due to the impression of the flat field on top of the image. The onboard ACQ background and flat-field images need to be reduced in a similar manner as performed by the FSW to achieve a meaningful comparison. The coronagraphic acquisition n4q832npq will be used as an example to demonstrate off-line processing.

The background image (n4q832npq_rwb.fits) must be subtracted from the image of the hole (n4q832npq_rwf.fits), and the resulting image flat fielded using a preflight flat or SMOV flat with the hole at a different position. In this example, the pre-flight flat field hls1337dn_flat.fits was used to process the hole image. The task **imcalc** is used to combine the pair of background and hole images, taking the minimum value at each pixel in order to eliminate cosmic rays.

```
> imcalc n4q832npq_rwb01.fits[1],n4q832npq_rwb02.fits[1] \
>>> min_bac "min(im1,im2)"

> imcalc n4q832npq_rwf01.fits[1],n4q832npq_rwf02.fits[1] \
>>> min_flat "min(im1,im2)"

> imarith min_flat - min_bac min_flat_bac
> imarith min_flat_bac * nref$hls1337dn_flat.fits[1] \
>>> pro_flat_bac
```

One can then invert the flat-fielded hole image to make the hole positive, and then use the **IRAF** task **center** to determine the centroid of the reversed hole image.

The position of the coronagraphic hole measured from the pipeline processed image is (73.384, 213.082), while the measured position of the hole from the off-line processed image is (73.273, 213.163). The difference is ~0.1 pixel in the x- and y-positions. This measured offset in hole position

is most probably due to the different calibrations performed on the ACQ images. The pipeline processed ACCUM images are not dark or background corrected. The location of the coronagraphic hole in the pipeline on-orbit flat was patched and could contribute to error in determining the position of the hole.

For comparison with the FSW determined position of the hole, the **IRAF** positions of the hole need to be converted into detector coordinates by subtracting them from 256.5. For example:

```
Hole:
NYHOLE = 256.5 - 73.273 = 183.227
NXHOLE = 256.5 - 213.163 = 43.337
```

In this example, for back-to-back orbit ACQ images n4q832npq and n4q833nzq (obtained prior to June 28, 1998), the difference between the two positions derived for the hole (**IRAF** and FSW) in detector coordinates is ~0.9 pixels in y and ~0.3 pixels in x. This is much larger than can be explained by summing the errors of the target and hole positions in quadrature, and is due to a bug in the early version of the FSW, which introduced errors in the derived hole positions.

Measuring the Target Position

The **IRAF** task **center** can be used to determine the centroid of the target in the NIC2 field of view. For comparison with the FSW positions of the target, the centroid values need to be converted into detector coordinates by subtracting them from 256.5. For example:

```
Star:
NXCENTER = 256.5 - 133.725 = 122.775
NYCENTER = 256.5 - 175.708 = 80.792
```

In this example, the target position we have measured agrees quite well with that determined by the FSW. The slight differences are most probably due to the different algorithms used to determine the centroids.

5.5.4 Recalibrating Coronagraphic Images

The user may wish to recalibrate coronagraphic data using the best reference files currently available (see Section 3.5). Unfortunately, at this time there are no standard dark reference files available from the calibration database for ACCUM and BRIGHTOBJ mode observations (see Section 4.2.3 for a discussion). Some coronagraphic observers obtained their own on-orbit ACCUM mode darks, which are available from


the *HST* Archive and can be used for calibrating the science data. If you have questions about calibrating coronagraphic ACCUM images, please contact the STScI help desk (help@stsci.edu).

Any given on-orbit flat-field observation with NIC2 will include the coronagraphic hole. Because the hole moved with time, it is unlikely that the hole will be in the same location for a given observation as it was in a flat-field taken at a different time. This can have particularly catastrophic consequences for coronagraphic data. It is therefore important to use a flat-field where the hole is in a substantially different location. For Cycle 7 and 7N, the pre-flight flat-fields from thermal vacuum testing show this feature and can be used (however, since the preflight flat-fields were obtained at a different temperature compared to on-orbit, they do not provide a perfect match). A flat-field where the hole has been "patched" can also be used. Patched flat-fields should be suitable for most purposes, although the patches are not perfect, and it is possible that small mismatches may still affect coronagraphic science. Both the pre NCS (patched and unpatched) and post NCS (only un-patched) flat-fields are available at the NICMOS Web page:

<http://www.stsci.edu/hst/observatory/cdbs/SIfileInfo/NICMOS/NICFlatReference>

Contemporary "Hole" Flats

Calibration using contemporary flat fields would remove the very strong hole-edge gradient resulting from calibration with a non-contemporaneous hole image or with a patched flat. The F160W filter acquisition lamp on/off paired images obtained as part of the Mode-2 target acquisition process can be used to create a flat-field reference file. The hole position in these images is at the same location as the hole position in the associated coronagraphic observations. Reference files created from these images would be appropriate for regions close to the coronagraphic hole. The S/N for these F160W filter reference files would be S/N ~100.



Note: the recommended standard calibration reference files have high S/N (typically ~ 1200) and should be used for regions far from the coronagraphic hole. The Mode-2 acquisition F160W filter lamp and background images will usually contain an overexposed image of the target.

For completeness, the following processing steps to create a contemporary flat field from the ACQ images are listed to assist the user.

```

ni> hedit n4xj13jwq_rwb.fits[0] flatcorr OMIT ver-
ni> hedit n4xj13jwq_rwb.fits[0] unitcorr PERFORM ver-
ni> hedit n4xj13jwq_rwb.fits[0] photcalc OMIT ver-

ni> hedit n4xj13jwq_rwf.fits[0] flatcorr OMIT ver-
ni> hedit n4xj13jwq_rwf.fits[0] unitcorr PERFORM ver-
ni> hedit n4xj13jwq_rwf.fits[0] photcalc OMIT ver-

ni> calnica n4xj13jwq_rwb.fits "" > n4xj13jwq_btrl.log
ni> calnica n4xj13jwq_rwf.fits "" > n4xj13jwq_ftrl.log

ni> mssplit n4xj13jwq_clb.fits
ni> mssplit n4xj13jwq_clf.fits

ni> mscombine n4xj13jwq_clb01.fits,n4xj13jwq_clb02.fits \
>>> n4xj13_bck
ni> mscombine n4xj13jwq_clf01.fits,n4xj13jwq_clf02.fits \
>>> n4xj13_lamp

ni> msarith n4xj13_lamp.fits - n4xj13_bck.fits \
>>> n4xj13_lamp_bck

ni> msstat n4xj13_lamp_bck.fits[sci,1][1:256,36:256]
ni> msarith n4xj13_lamp_bck.fits / 1169.64 norm_lamp_bck

ni> msarith 1.0 / norm_lamp_bck n4xj13_f160wflt
ni> hedit n4xj13_f160wflt.fits[0] PEDIGREE \
>>> "Contemporary 31/08/98" add+

```

Recalibrating the ACQ ACCUM Images

Some observers have expressed the desire to obtain photometry from the ACQ images of their targets. These images are not dark corrected and will need to be recalibrated. As discussed in Section 4.2.3, however, at the present time there are no standard dark reference files for ACCUM mode images. Appropriate DARK exposures matching the ACQ image exposure times may be available in the *HST* Archive. If you are a NICMOS GO, please speak with your contact scientist (CS) about dark subtraction for ACCUM images, or contact help@stsci.edu.

We note here that due to a software bug, the exposure time stated in the header keyword EXPTIME is in error for ACQ data taken prior to October

19, 1998. The commanded exposure time listed in the SHP and UDL data file (`_spt.fits`) should be used for photometry. For example:

```
> hedit n4xj13jwq_raw.fits[0] EXPTIME .
n4xj13jwq_raw.fits[0],EXPTIME = 0.625648

> hedit n4xj13jwq_spt.fits[0] CMD_EXP .
n4xj13jwq_spt.fits[0],CMD_EXP = 0.255647987127
```

The SAMPTIME keywords have to be changed in both SCIENCE groups of the raw, uncalibrated imageset (`_raw.fits`) before **calnica** processing.

5.5.5 Reducing and Co-adding Coronagraphic Images

The OPUS pipeline will combine multiple coronagraphic exposures using **calnicb**. This can cause difficulties, however, for coronagraphic data analysis. If the individual images that form a mosaic require registration, some smoothing will be introduced by the bi-linear interpolation that is used by **calnicb** to shift the images. Even if the images are well registered to begin with, slight differences in the diffraction pattern due to movement of the coronagraphic hole may cause the **calnicb** cross-correlation routine to compute non-zero offsets between the various images. This will lead to misregistration and again, some smoothing. One way around this problem is to force **calnicb** not to shift any of the images before averaging them together. This can be accomplished by adding columns of XOFFSET and YOFFSET values to the input association table (`_asn.fits`) used by **calnicb** and setting their data values to zero. However, in general, PSF subtraction is best performed with individual images and not with the mosaic image.

Pedestal Removal

The residual bias or “pedestal” effect was described in Section 4.2.2, and should be removed if possible before analyzing coronagraphic data. The **pedsky** task described in Section 4.2.4 may not be suitable for coronagraphic images where a bright object dominates the field of view. In this case, the **pedsub** task may be more appropriate. This method has been used successfully with coronagraphic images from the SMOV calibration program 7052 (1997 July 23). The **pedsub** task was run with the parameters `filter=mask` (i.e., applies unsharp-masking filter to remove low spatial frequency information) and `doquadeq=no` (i.e., do not force quadrant boundaries to be continuous). The images of the stellar PSF in the coronagraphic images of the 7052 data fill the quadrant with the coronagraphic hole and spill over into adjacent quadrants. This constrains

the determination of the pedestal contribution in that quadrant. A mask file was created to flag bright pixels (threshold limit= 4.0 cts/sec); the flagged pixels were not used for estimating the pedestal contribution. This mask was added to the mask of known bad pixels included in the DQ image extension, and the **pedsub** parameters **dqon** and **dqpar** were used to tell the task which mask values correspond to pixels that should be ignored when fitting the pedestal.

Removing Other Image Artifacts

The identification and removal of bad pixels, “grot,” and other NICMOS data anomalies are discussed in Chapter 4. For coronagraphic data, the presence of a bright source commonly induces the vertical streaks known as the “Mr. Staypuft” effect (see Section 4.8.4). Because of the bright coronagraphic target, it is not possible to fit simple medians to columns along the entire y-axis length of the image in order to measure and subtract the Mr. Staypuft streaks. It may be possible to remove (or at least reduce) the streaks using a correction image derived from the bottom rows of the image only, far from the coronagraphic target. The first 19 rows are usually the only area of the image that is not intersected by the bright diagonal diffraction spike emanating from the hole. You may use **blkavg** to average the first 19 rows, and then **blkrep** to “stretch” this row average to form a 2-dimensional image to be subtracted from your data. Care must be taken to ensure that bad pixels (hot or cold pixels, or “grot”) do not bias the row average: if necessary, interpolate over bad pixels using **fixpix**.


```
> blkavg n4q810csq_cal.fits[1:256,1:19] n4q810csq_line\
>>> op=ave

blocking factor in dimension 1 (x or column) (1:) (1):
blocking factor in dimension 2 (y or line) (1:) (121):

> blkrep n4q810csq_line n4q810csq_area 1 256

> imarith n4q810csq_cal.fits[1] - n4q810csq_area.hhh\
>>> n4q810csq_snb
```

Figure 5.9: Coronagraphic image, F110W filter.

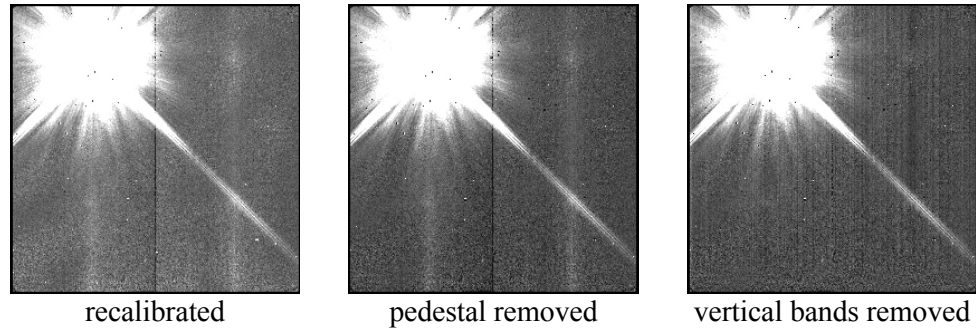

Star centered in hole with image recalibrated (left), pedestal removed (middle), and with “Mr. Staypuft” striping partially corrected (right). Images are displayed with the same stretch

In Figure 5.9 above, the correction for the Mr. Staypuft bands is not perfect, and shows the limitations of doing this. The amplitude may modulate from one quadrant to another for electronic reasons, and flat fielding also introduces variations along the column so that a constant correction derived from the bottom rows may not be appropriate. Nevertheless, the process results in first-order cosmetic improvement, and may be worthwhile.

Persistent afterimages from previous exposures of the target star (see Section 4.8.1) can also be a problem for coronagraphic images, and users should be aware of this effect.

PSF Subtraction

The light distribution within the PSF and the pattern of light scattered about the hole can change significantly on both short and long time scales, from orbit to orbit and over the lifetime of NICMOS (see Section 5.4 for a general discussion of focus and PSF issues). These changes may be attributed to several factors, including OTA focus variations, thermally induced motions in NICMOS fore-optics, possible changes in the position of the cold mask, and coronagraphic hole motion. All of these changes are related to either the thermal input to the telescope, changes in Sun angle (attitude) and spacecraft roll, or to the dewar thermal short. The PSF also varies as a function of position across the field of view, which may affect the quality of PSF subtractions (see Figure 5.10). In addition, the *HST* focus position is known to oscillate with a period of one *HST* orbit. Changes in the focus position are attributed to thermal contraction/expansion of the optical telescope assembly (OTA) resulting from the telescope warm up and cool down during an orbital period.⁵ These short term focus position variations are usually referred to as “OTA breathing”, “*HST* breathing”, “focus breathing”, or simply “breathing”.

5. NICMOS Instrument Science Report, [NICMOS ISR-98-015](#)

During Cycle 7 and 7N, the NICMOS dewar anomaly caused the coronagraphic hole to migrate to different locations on the detector. The position of the hole on the detector had been observed to move as much as ~ 0.25 pixel in three orbits. The movement of the hole was found not to be uni-directional, but rather, the hole “jitters” back and forth along an X-Y diagonal by as much as ± 0.5 pixel.⁶

The direct subtraction of two unregistered coronagraphic images that were not obtained back-to-back in the same orbit with a change in roll can yield large residuals. Coronagraphic images need to be subpixel shifted and/or convolved with a Gaussian function to match the observed PSF before subtraction.


The following discussion applies both subpixel shifting and Gaussian convolution reduction techniques to two F110W filter images from the NICMOS calibration program 7052. The data used in the examples below are n45j22lam and n45j23mym. The data were obtained in consecutive orbits with a spacecraft roll of 36° between orbits.

Subpixel Shifting

The images to be subtracted must be registered to sub-pixel accuracy in order to achieve good results. The **IRAF** task **xregister** provides one way to determine the offsets between the images, and to shift one into alignment with the other. For the example considered here, a 995 pixel region ([27:121,162:256]) around the hole was used as the area for cross-correlation, and a shift of $dx = -0.286$, $dy = 0.136$ pixels was measured between the images. The example shown in Figure 5.10 and Figure 5.11 displays the subtraction of the two images, using both unregistered (left) and registered (right) data. The subtraction using the registered images exhibits a more symmetrical residual light pattern about the hole. Occasionally, cross correlation does not yield the best measure of the image offsets. You may find that “trial-and-error” shifting by various fractional pixel amounts, minimizing the subtraction residuals “by eye,” can yield the best results.

6. NICMOS [ISR 98-012](#).

Figure 5.10: PSF Subtraction.

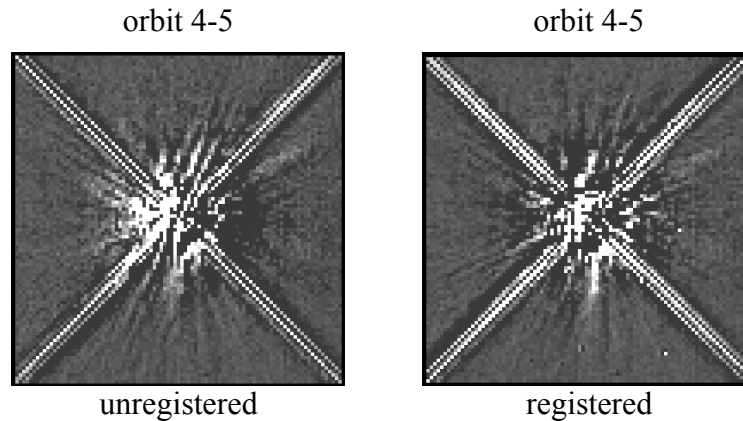


F110W filter images obtained in back-to-back orbits with a roll of the spacecraft between orbits. Direct subtraction of images (left) and a subtraction with the second image shifted to match the first image (right).

Gaussian Convolution

The interpolation introduced by sub-pixel shifting has the effect of smoothing the image slightly. Subtracting the blurred image from the unblurred image has the effect of edge enhancement. One way to suppress high frequency variations in the images is to convolve one or both by a Gaussian filter. This may help reduce residuals in the subtracted image. The **IRAF** task **gauss** may be used to smooth the images. The resulting images for two different convolutions, with $\sigma = 0.4$ and $\sigma = 0.8$, are presented in Figure 5.11.

Figure 5.11: PSF Subtraction.

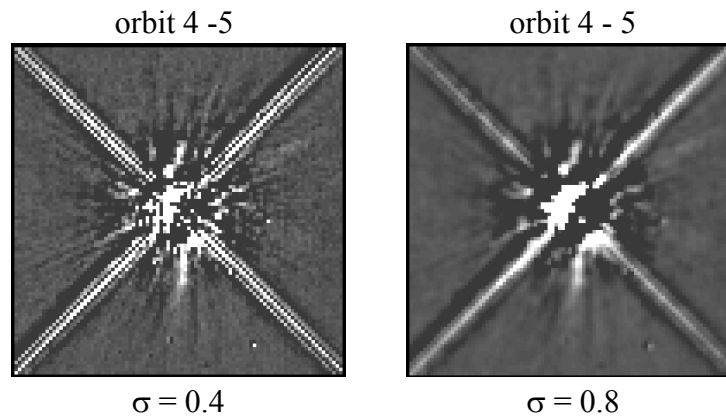

F110W filter images obtained in back-to-back orbits with a roll of the spacecraft between orbits. Images convolved with a Gaussian function, $\sigma = 0.4$ (left) and $\sigma = 0.8$ (right) and subtracted.

In this example, the $\sigma = 0.4$ convolution results in a slight improvement over the subtractions shown in Figure 5.10. Possibly, this choice is

undersmoothing the data. The $\sigma = 0.8$ convolution more closely matches the low frequency components. Determining a suitable degree of smoothing will require experimentation by the user.

5.6 Analysis of Polarization Images

5.6.1 Introduction

The filter wheels of cameras NIC1 and NIC2 each contain three polarizing filters with unique polarizing efficiencies and position angle offsets. The original design specified that the position angle of the primary axis of each polarizer (as projected onto the detector) be offset by 120° from its neighbor, and that the polarizers have identical efficiencies. While this clean concept was not strictly achieved in NICMOS, the reduction techniques described below permit accurate polarimetry using both cameras over their full fields of view.

A complete set of polarimetric observations will contain images obtained in all three polarizers of the selected wavelength range. We assume that each image has been processed through **calnica** and **calnicb** to produce a fully reduced and (if necessary) mosaiced image in each of the three filters, with the data corrected for saturation and cosmic rays and converted to flux density using the appropriate photometric calibration constants for the polarizers.

To generate Stokes parameters, the relative differences in flux between images in the different polarizing filters are used. Where the signal level is very faint, and the signal-to-noise ratio is very low, the differences may be very large but dominated by noise. If you attempt to calculate the Stokes parameters using such data, you will likely obtain large and entirely spurious polarizations. Therefore, it is not advisable to use low signal-to-noise data to calculate polarization. To avoid this problem, it is suggested to estimate the noise in an area of the image free of sources, and then set a threshold at a value of order five to ten times this noise level. Using the **IRAF** task **imreplace**, all pixels with signals below this threshold should be set to some arbitrary value, probably close to the measured noise level. This action will cause all areas of the image where the signal level is very faint to show zero polarization. To further increase signal-to-noise, bin the data in each of the three images before computing the Stokes parameters. Once the parameters have been derived, clipping the

Q and U images at ± 1 and the polarization intensity image at values < 0 or > 1 will also help in increasing the signal-to-noise.



“Analysis of Polarized Light with NICMOS” by Hines, Schmidt & Schneider (2000, PASP, 112, 983) is a highly valuable reference discussing NICMOS polarimetric measurements and data analysis.

5.6.2 Theory

In order to reduce data obtained with a set of polarizers, three quantities are needed. They are the throughput for unpolarized light, the efficiency of the element as a polarizer, and the orientation of the polarizer. These quantities can be expressed in a polarization reduction algorithm to form a solution containing the polarization characteristics of the incoming beam (i.e., the Stokes parameters I , Q , and U).

The general form of the equation for polarimetric data reduction is expressed as

$$I'_k = A_k I + \varepsilon_k (B_k Q + C_k U)$$

where I'_k is the emerging light intensity from the k th polarizer, A_k , B_k and C_k are the transmission coefficients, and ε_k is the polarizing efficiency.⁷ This linear equation captures the observed signal from a polarized source of intensity I and linear Stokes parameters Q and U , which describe the state of polarization for the target object. The above equation reduces to a set of three equations with three unknowns. The solution results in the Stokes parameters for the incoming light.

For NICMOS the transmission coefficients are⁸

$$A_k = \frac{(t_k)}{2} (1 + l_k), \quad B_k = \frac{1 - l_k}{1 + l_k} \cos 2\phi_k, \quad C_k = \frac{1 - l_k}{1 + l_k} \sin 2\phi_k$$

where ϕ_k is the position angle of the k th polarizer relative to the NICMOS entrance aperture, t_k is the fraction of light transmitted for a 100% polarized input aligned with the polarizer's axis, and l_k is the fraction transmitted when the incoming light is perpendicular to the axis of the polarizer.

7. Polarizer efficiency is defined as $\varepsilon = (S_{par} - S_{perp}) / \langle S_{par} + S_{perp} \rangle$ where S_{par} and S_{perp} are the respective measured signals for a polarizer oriented parallel and perpendicular to the axis of a fully polarized beam.

8. For further detailed information on the derivation of the coefficient matrices, see Hines, D.C. “Imaging Polarimetry with NICMOS”, VLT Conference 1998.



For NICMOS, the observed signal from a polarized source of total intensity I contains an added term in the transmission coefficients, namely $0.5(1 + I_k)$.

Table 5.7 and Table 5.8 below present respectively the properties of the individual polarizers for Cycle 7/7N and Cycles 11 and beyond. The Cycle 11 and beyond properties have been reduced by Batchelor et al. (2009, PASP, 121, 153). Therefore the values in Table 5.8 and the post-NCS coefficient matrices, supersede values given in earlier versions of the Data Handbook.

Table 5.7: NIC1 & NIC2 Polarizer Properties

NIC 1 (Cycle 7)					NIC 2 (Cycle 7)				
Filter	ϕ_k	ϵ_k	t_k	I_k	Filter	ϕ_k	ϵ_k	t_k	I_k
POL0S	1.42	0.9717	0.7760	0.0144	POL0L	8.84	0.7313	0.8981	0.1552
POL120S	116.30	0.4771	0.5946	0.3540	POL120L	131.42	0.6288	0.8851	0.2279
POL240S	258.72	0.7682	0.7169	0.1311	POL240L	248.18	0.8738	0.9667	0.0673

The resulting Cycle 7/7N coefficient matrices become⁹

$$M_{NIC1} = \begin{bmatrix} 0.3936 & 0.3820 & 0.0189 \\ 0.4025 & -0.1166 & -0.1526 \\ 0.4054 & -0.2876 & 0.1195 \end{bmatrix}, \quad M_{NIC2} = \begin{bmatrix} 0.5187 & 0.3614 & 0.1152 \\ 0.5250 & -0.0411 & -0.3276 \\ 0.5159 & -0.3262 & 0.3111 \end{bmatrix}$$

which can be used to compute the expected (I_1 , I_2 , I_3) for a given set (I , Q , U). By inverting the appropriate matrix, the Stokes parameters (I , Q , U) can be computed from a set of observations (I_1 , I_2 , I_3).

9. Further detailed information on calibration methodologies and transformations between different polarizers, see Mazzuca, Sparks, Axon, NICMOS [ISR 98-017](#), “Methodologies to Calibrating NICMOS Polarimetry Characteristics, 1998 (computed from equation 27) of Mazzuca et al 1998.

Table 5.8: NIC1 & NIC2 Polarizer Properties for Cycle 11 and Beyond

NIC 1 (Cycle 11 and beyond)					NIC 2 (Cycle 11 and beyond)				
Filter	ϕ_k	ε_k	t_k	l_k	Filter	ϕ_k	ε_k	t_k	l_k
POL0S	1.42	0.9717	0.7760	0.0144	POL0L	8.84	0.7313	0.882	0.1552
POL120S	116.30	0.4771	0.57	0.3540	POL120L	131.42	0.6288	0.837	0.2279
POL240S	258.72	0.7682	0.69	0.1311	POL240L	248.18	0.8738	0.9667	0.0673

The resulting coefficient matrices for post-NCS data become

$$M_{NIC1} = \begin{bmatrix} 0.3936 & 0.3820 & 0.0189 \\ 0.3859 & -0.1118 & -0.1463 \\ 0.3902 & -0.2768 & 0.1150 \end{bmatrix}, \quad M_{NIC2} = \begin{bmatrix} 0.5094 & 0.3550 & 0.1131 \\ 0.5139 & -0.0403 & -0.3206 \\ 0.5159 & -0.3262 & 0.3111 \end{bmatrix}$$

The errors on the Stokes parameters are determined by straightforward propagation of errors,

$$\sigma_{S_i}^2 = \sigma_{I_1^*}^2 \left(\frac{\partial S_i}{\partial I_1^*} \right)^2 + \sigma_{I_2^*}^2 \left(\frac{\partial S_i}{\partial I_2^*} \right)^2 + \sigma_{I_3^*}^2 \left(\frac{\partial S_i}{\partial I_3^*} \right)^2$$

where S_k represents an incoming Stokes vector, and I_k^* defines the set of three observed intensities. Therefore,

$$\begin{aligned} \sigma_I^2 &= a_{11}^2 \cdot \sigma_{I_1^*}^2 + a_{12}^2 \cdot \sigma_{I_2^*}^2 + a_{13}^2 \cdot \sigma_{I_3^*}^2 \\ \sigma_Q^2 &= a_{21}^2 \cdot \sigma_{I_1^*}^2 + a_{22}^2 \cdot \sigma_{I_2^*}^2 + a_{23}^2 \cdot \sigma_{I_3^*}^2 \\ \sigma_U^2 &= a_{31}^2 \cdot \sigma_{I_1^*}^2 + a_{32}^2 \cdot \sigma_{I_2^*}^2 + a_{33}^2 \cdot \sigma_{I_3^*}^2 \end{aligned}$$

where a_{ij} represents the elements of the inverted transmission coefficients matrix.

The Stokes parameters can then be combined to yield the polarized intensity,

$$I_p = \sqrt{(Q^2 + U^2)}$$

as well as the degree of polarization P and the position angle of polarization θ_p , where

$$P = \frac{I_p}{I}, \quad \theta_p = \frac{1}{2} \text{atan} \frac{U}{Q}$$

Because the polarizers are non-ideal, I , Q , and U are correlated when calculating P and θ_p . Therefore, covariance must be taken into account when calculating the errors.

For the degree of polarization, the covariance is

$$\begin{aligned} \sigma_{P^2} = & \sigma_I^2 \left(\frac{\partial P}{\partial I} \right)^2 + \sigma_Q^2 \left(\frac{\partial P}{\partial Q} \right)^2 + \sigma_U^2 \left(\frac{\partial P}{\partial U} \right)^2 + \\ & 2\sigma_{IQ} \left(\frac{\partial P}{\partial I} \right) \left(\frac{\partial P}{\partial Q} \right) + 2\sigma_{IU} \left(\frac{\partial P}{\partial I} \right) \left(\frac{\partial P}{\partial U} \right) + 2\sigma_{QU} \left(\frac{\partial P}{\partial Q} \right) \left(\frac{\partial P}{\partial U} \right) \end{aligned}$$

where

$$\frac{\partial P}{\partial I} = \frac{\sqrt{Q^2 + U^2}}{I^2}, \quad \frac{\partial P}{\partial Q} = \frac{Q}{I\sqrt{Q^2 + U^2}}, \quad \text{and} \quad \frac{\partial P}{\partial U} = \frac{U}{I\sqrt{Q^2 + U^2}}$$

The covariance for the position angle is

$$\sigma_{\phi_p}^2 = \sigma_Q^2 \left(\frac{\partial \phi_p}{\partial Q} \right)^2 + \sigma_U^2 \left(\frac{\partial \phi_p}{\partial U} \right)^2 + 2\sigma_{QU} \left(\frac{\partial \phi_p}{\partial Q} \right) \left(\frac{\partial \phi_p}{\partial U} \right)$$

where

$$\frac{\partial \phi_p}{\partial Q} = \frac{U}{2 \left(\frac{U^2}{Q^2} + 1 \right) Q^2}, \quad \frac{\partial \phi_p}{\partial U} = \frac{1}{2 \left(\frac{U^2}{Q^2} + 1 \right) Q}$$

5.6.3 A Useful Script for Polarization Analysis

An interactive IDL program to derive relevant parameters from NICMOS polarization images has been developed. The IDL program reads three images taken with three polarizers from NIC1 or NIC2 produces five images as output. The output images are:

- *q.fit* and *u.fit*, two images representing the Stokes parameters,

- *i.fit*, the total intensity,
- *p.fit*, the degree of polarization, and
- *theta.fit*, the polarization angle.

Polarization vectors or contour maps can be superimposed over the intensity image. The program is available from the STScI NICMOS Web site under [software tools](#), and is described in more detail in Mazzuca & Hines, NICMOS [ISR 99-004](#), “User’s Guide to Polarimetric Imaging Tools.” For news and updates on this tool, see the NICMOS Web page:

http://www.stsci.edu/hst/nicmos/performance/polarimetry/nicmos_polar.html/

5.7 Grism Data Reduction

The NICMOS camera 3 grisms permit multi-object, slitless, low resolution spectroscopy. The reduction and analysis of NICMOS grism data benefit from decisions made by the user and from careful, interactive examination, and are therefore discussed here rather than in the chapter on pipeline calibration.

Software to extract spectra from NICMOS grism images has been developed at Space Telescope European Coordinating Facility (ST-ECF). Two packages are available: **NICMOSlook**, which is interactive, and **aXe**, which is non-interactive. The interactive program, **NICMOSlook**, provides a number of tools called from an IDL GUI widget. This program is recommended for most extraction because of its versatility and interactive features. The automatic version, **aXe**, is recommended if an extraction of a large number of spectra from different images is desired. Both software packages, together with user documentation, can be obtained from the [ST-ECF Web](#) site. Here we offer only a brief description of grism analysis methodology, and refer the user to the documentation provided with the software for details. The ST-ECF also maintains grism calibration reference files which are included with the software distributions.

The extraction software assumes that grism data are pipeline processed like regular images with the exception that they are not flat fielded by **calnica**. The flat-field correction for a given pixel depends both on the pixel location (x,y) and on the wavelength of the light which is dispersed onto that pixel. The latter is not known until the location of the dispersed source has been specified, and therefore the flat fielding cannot be done in advance. It is omitted during 2 dimensional data processing through **calnica**. Later, after 1-dimensional spectra have been extracted from the grism images, the

extraction software applies a wavelength dependent correction for QE variations (see Section 5.8.2).

The wavelength calibration for the extraction of spectra requires a direct image corresponding to each grism image. If individual exposures for the grism images are co-added before extraction, a similar co-addition should also be performed for the direct images in order to maintain the relative position of objects in the direct image with the corresponding spectrum in the grism image. If grism and direct images are processed separately by **calnicb**, this relative registration is, in general, not maintained.



In general, combining dithered grism images before extracting spectra is probably not a good idea whenever it can be avoided. As noted above, every pixel on the array has a different spectral response. Combining dithered grism images before extraction will combined data from different pixels, making it difficult or impossible to reliably flux calibrate the resulting spectrum. In general, we recommend to feed individual images direct from calnica to the extraction software.

5.7.1 Extraction Software

Detailed software manuals and descriptions of the extraction algorithms can be found at:

<http://www.stecf.org/instruments/NICMOSgrism/>.

Only a brief summary is given below.

Input Files

The extraction software requires two types of input images, one for object finding, and one which contains the spectra to be extracted. Typically, the former is a direct image of the target field obtained with one of the NICMOS continuum filters, preferably at a wavelength within the range covered by the grism. However, the grism image itself can also be used for object finding, e.g. on the zeroth order spectra. The image which contains the spectra is assumed to be not flat fielded, which is the default in **calnica**.

In most cases, the input files are the output of **calnica** (*_cal.fits). The software packages also accept plain FITS images without NICMOS specific extensions, but some functionalities which depend on the error planes (*_cal.fits[err]) or data quality flags (*_cal.fits[dq]) will not be available.

Output Files

The basic output of the extraction are the spectra, which can be written as ASCII or FITS tables, and associated metadata.

5.7.2 Processing

Object Detection and Classification

The extraction software programs include automatic finding of objects on the direct images. **NICMOSlook** uses **DAOFIND** for that purpose, while **aXe** uses **Sextractor** to find and classify objects. In **NICMOSlook**, objects can also be marked interactively with the cursor.

It may sometimes be useful to use the grism images to search for particular types of spectra “by eye”. In this case, the spectral images can be flat fielded using ordinary, on-orbit grism flat fields, displayed, and examined visually for e.g. emission line objects, or very red spectra. Ordinarily, these on-orbit flat fields are *not* used as part of NICMOS grism data processing: instead, the flat fielding is done on the extracted spectra, as is described below. Once the interesting objects have been identified, their spectra should be extracted from non flat-fielded grism images.

Location of Spectra

The positions of the direct objects can be used to compute the location and orientation of the spectra. The software packages know the approximate position of spectra relative to the position of the object on the direct image. However, the orientation of spectra varies enough from observation to observation so that a “tracing” of spectra is necessary for accurate spectrum extraction. See the **NICMOSlook** manual for details.

Background Subtraction

After source identification, an estimate of the two-dimensional background level is derived and removed from each image.

The grism image is not flat-fielded and the QE variations across the NICMOS detectors are strong, implying that a significant structure is present in an image of blank sky. Several options to subtract this background are provided. They include interpolation over the region of the spectra, or subtracting scaled versions of background images. The extraction software determines the regions of interpolation excluding positions occupied by other spectra in the image. The most accurate background subtraction can be achieved if a background image is specially prepared “by hand” from a dithered dataset.

Extraction of Spectra

Flux and Error Bars

Once objects on the images have been detected, their spectra can be extracted. The flux is then given by:

$$F_j = \sum_i w_{ji} g_{ji}$$

where the sum over the flux g_{ji} of all pixels at wavelength λ is performed with weights w_{ji} .

Several options for the weights can be used to achieve optimum S/N. Constant weights lead to an optimum extraction for high S/N spectra, while for background limited objects, weights can be derived from the profile of the spectrum to be extracted. The profile can either be determined directly from the spectrum, or predicted from the direct image for very low S/N spectra under the assumption that the shape of the object is independent of wavelength. First, the size and orientation of the object is computed from the direct image.



Since NICMOS grism images are undersampled, spectra of point sources and sources up to the size of a few pixels are best extracted using constant weights even for low S/N spectra.

The error estimate e_{ji} for each pixel is propagated from the ERR array of the input grism image. The error estimate e_j for each wavelength is then the weighted quadratic sum over the errors of all pixels at constant wavelength.

Wavelength Calibration

The dispersion relation and the deviation of the spectra have been determined from wavelength calibration observations, and are parametrized as:

$$\lambda = a_0 + a_1 x + a_2 x^2 + a_3 x^3$$

where x is the deflection in pixels relative to the position of the object in the direct image and λ is the corresponding wavelength. The coefficients are contained in the reference file `grismspec.dat` for **NICMOSlook** or in the configuration file (`.conf`) for **aXe**. The dispersion relation is given by:

$$\Delta y = b_0 + b_1 r + b_2 r^2 + b_3 r^3$$

where r is the distance of a pixel (x, y) from the object of coordinates (x_o, y_o) and Δy is the deviation in pixels of the spectrum from a horizontal line. The alignment of the spectrum is taken into account by rotating the

grism image around the object position (x_o, y_o) prior to the extraction. The distortions in the spectra are taken into account by introducing a corresponding distortion in the weights used for the extraction. For results from recent grism wave-length calibrations. For further updates please refer to the NICMOS Web page at:

<http://www.stsci.edu/hst/nicmos>

Flat Fielding of Spectra

After the spectra are extracted, the fluxes are corrected for pixel-to-pixel variations in the quantum efficiency of the detector (i.e., flat fielded). The QE variations depend both on the wavelength and on the position of the object on the detector. Because of this wavelength dependence, the flat fielding cannot be performed before the spectra are extracted and wavelength calibrated. The corrected flux $f_c(\lambda)$ is computed as follows

$$f_c(x,y) = f(x,y)q(x,y,\lambda)$$

where $q(x,y,\lambda)$ are interpolated flat fields. For wavelengths where narrow band flat fields are available, they are used. For other wavelengths, the correction factors are derived through interpolation from a set of monochromatic flat-field images (see Storrs et al. 1999, NICMOS [ISR-99-002](#)). The filters used in this process are F108N, F113N, F164N, F166N, F187N, F190N, F196N, F200N, F212N, F215N, and F240M. The most recent flat-field reference files are available at [NICMOS dynamic reference files Web](#) pages.

Flux calibration and Correction for Pixel Response Function

Once the spectra are extracted, the count rates in ADU/second are converted to physical units using calibration data from photometric standards P330E and G191B2B.

Undersampling of NICMOS grism images in combination with significant variation of the QE across any given pixel imposes a wave-like pattern onto extracted spectra of point sources and small objects. Since spectra are not exactly aligned with the rows of the images, the exact sub-pixel position and orientation of the spectra determines the phase and period of those waves. A simple model can be used to correct this effect for point sources. Details are discussed in an article by W. Freudig in the May 1999 issue of the ST-ECF Newsletter.

Deblending of Overlapping Spectra

Since the NICMOS gratings are slitless, overlaps among different spectra are likely to happen. The strategy of observing the same target at different telescope roll angles helps remove overlap in many instances.

aXe reports an estimate of the contamination by nearby objects. **NICMOSlook** includes an algorithm designed to remove or minimize contamination of one spectrum from another. The deblending algorithm is described in detail in the **NICMOSlook** software manual. The basic

requirement for the algorithm to work is that, at each wavelength, different spatial portions of the spectrum to be deblended have different levels of contamination. The deblending algorithm relies on the assumption that the shape of the object is the same at all wavelengths.

Index

A

- absolute photometry 135
- absolute spectrophotometry
 - grism 136
- ACCUM mode 5
- algorithm
 - calnica 41
 - calnicb 56, 58
- amplifier glow 76
- analog-to-digital conversion 45
- aperture correction 133
- array readout 4
- association table 11, 17
- astrometry
 - absolute 141

B

- background 54, 61
- bars 91
- bias
 - bias reset level 77
 - jumps 81
 - pedestal 79
 - shading 77
- bias correction 45
- bias derived temperature
 - CalTempFromBias 37, 39
- Bright Earth Persistence (BEP) 55, 109
 - nic_rem_persist 55
- BRIGHTOBJ mode 6

C

- calibrated science file 11
- calibration 41, 56
 - re-calibrating, when to 62

- switches 64
- calnica task
 - algorithm 41
- calnicb task
 - algorithm 56
- CalTempFromBias
 - bias derived temperature 37, 39
- chcalpar task
 - calibration switches 64
- chop pattern
 - background 61
- conversion
 - counts to flux or magnitude 124
- coronagraphic hole 103
- coronagraphic reductions 148
- cosmic ray identification 53
- cosmic ray persistence
 - see also saaclean 106
- count rate non-linearity 96

D

- dark current 74
- dark subtraction 48
- Data Quality Array
 - bit settings 15
- dataset 10
- differential photometry 130
- digiphot package
 - PSF subtraction 142
- distortion
 - geometric 138
- dither pattern
 - background 61

E

earthlight
 scattered 115
 emission line
 filters 135
 erratic middle column/row 103
 exposure log sheet 31
 exposures
 multiple, combining 60

F

files
 naming conventions 9
 filters
 available 3
 flat field
 color dependence 100
 flatcorr 51
 temperature-dependent 99

G

geometric distortion 138
 ghost
 optical 112
 grism
 absolute spectrophotometry 136
 aXe 39
 data reduction 167
 NICMOSlook 38
 spectroscopy 38
 grot 101

H

header keywords 19

I

icons
 used in this manual xii
 imheader task
 examine NICMOS header 29
 iminfo task
 examine NICMOS header 28
 integration 4
 intermediate multiaccum science file 11

K

keywords
 header 19

L

linearization correction 49

M

magnitude
 Janskys, NICMOS data 134
 markdq task
 mark data quality flags 120
 mode
 readout 4
 mosaic
 constructing 61
 mosaic file 11
 mstools package
 image sets 119
 MULTIACCUM mode 5
 MultiDrizzle 56
 multiple exposures
 combining 60

N**NICMOS**

absolute photometry 135
 ACCUM mode 5
 association table 17
 bad pixel 45
 BRIGHTOBJ mode 6
 calibration process 63
 described 2
 emission line filters 135
 file names 9
 grism spectroscopy 38
 grism, absolute spectrophotometry 136
 keywords 19
 MULTIACCUM mode 5
 paper products 33
 pipeline calibration 35
 PSF, subtracting 141
 RAMP mode 7
 readout mode 4
 recalibrating data 62
 red leak 134

noise calculation 46

nonlinearity
detector 93

P

paper products 33

pedsky 87

pedsub 89

persistence
bright earth 109
cosmic ray 106
photon 105

Phase II
see "proposal"

photometric correction 52, 124

photometry
absolute 135
differential 130
pixel centering 131

photon persistence 105

pipeline
NICMOS calibration 35

pixel
bad 45
centering 131
hot, cold, grot 101

polarization
analysis 162

polarizer 3

post-calibration association table 11

proposal
comparing to data 31

PSF
NICMOS, subtracting 141

pstack task
plot samples as function of time 120

R

RAMP mode 7

raw science file 10

readout
mode 4

red leak 134

rnlinco 97, 122

runcalsaa 54

S

SAAClean 54, 106

scattered earthlight 115

spectra
extraction, grism 170

spectroscopy
grism 38

Staypuft (Mr. Staypuft anomaly) 110

STSDAS
NICMOS calibration 36
NICMOS software 119
support file 10, 18

T

trailer file 11, 18

typographic conventions
in this manual xii

U

units
conversion 124
user support
help desk ii

V

vignetting 104

W

warning
types in this document xii
wavelength
calibration, grism 170

Z

zeroth read
non-zero 134
zeroth read subtraction 45