



## 12724 - COS NUV Detector Recovery After Anomalous Shutdown

Cycle: 19, Proposal Category: CAL/COS

(Availability Mode: RESTRICTED)

### INVESTIGATORS

<i>Name</i>	<i>Institution</i>	<i>E-Mail</i>
<b>Mr. Thomas Wheeler (PI) (Contact)</b>	<b>Space Telescope Science Institute</b>	<b>wheeler@stsci.edu</b>
Dr. Alan D. Welty (CoI)	Space Telescope Science Institute	welty@stsci.edu

### VISITS

<i>Visit</i>	<i>Targets used in Visit</i>	<i>Configurations used in Visit</i>	<i>Orbits Used</i>	<i>Last Orbit Planner Run</i>	<i>OP Current with Visit?</i>
01	DARK	S/C	1	20-Jun-2012 21:02:45.0	yes
02	DARK	COS/NUV S/C	1	20-Jun-2012 21:02:53.0	yes
03	DARK	COS/NUV S/C	1	20-Jun-2012 21:03:00.0	yes
04	DARK DEUTERIUM	COS/NUV S/C	1	20-Jun-2012 21:03:03.0	yes
11	DARK	S/C	1	20-Jun-2012 21:03:06.0	yes
12	DARK	COS/NUV S/C	1	20-Jun-2012 21:03:11.0	yes
13	DARK	COS/NUV S/C	1	20-Jun-2012 21:03:17.0	yes
14	DARK DEUTERIUM	COS/NUV S/C	1	20-Jun-2012 21:03:21.0	yes

8 Total Orbits Used

## **ABSTRACT**

This proposal is designed to permit a safe and orderly recovery of the NUV-MAMA detector after an anomalous shutdown. This is accomplished by using slower-than-normal MCP high-voltage ramp-ups and diagnostics. Anomalous shutdowns can occur because of bright object violations, which trigger the Global Hardware Monitor or the Global Software Monitor. Anomalous shutdowns can also occur because of MAMA hardware anomalies or failures. The cause of the shutdown should be thoroughly investigated and understood prior to recovery. Twenty-four hour wait intervals are required after each test for MCP gas desorption and data analysis. Event flag 2 is used to prevent inadvertent MAMA usage.

The recovery procedure consists of four separate tests (i.e. visits) to check the MAMA's health after an anomalous shutdown: signal processing electronics check, slow, intermediate voltage high-voltage ramp-up, ramp-up to full operating voltage, and fold analysis test (See COS TIR 2010-01). Each must be successfully completed before proceeding onto the next. This proposal executes the same steps as Cycle 18 proposal 12430.

## **OBSERVING DESCRIPTION**

Anomalous shutdowns can occur because of bright object violations, which trigger the Global Hardware Monitor or the Global Software Monitor. Anomalous shutdowns can also occur because of MAMA hardware anomalies or failures. The cause of the shutdown should be thoroughly investigated and understood prior to recovery. Twenty-four hour wait intervals are required after each test for MCP gas desorption and data analysis. Event flags are used to prevent inadvertent MAMA usage.

The recovery procedure consists of four separate tests (i.e. visits) to check the MAMA's health after an anomalous shutdown. Each must be successfully completed before proceeding onto the next. This proposal executes the same steps as Cycle 18 proposal 12430.

- (1) Signal processing electronics check. The amplifier threshold voltage is reduced from 0.48V to 0.28V; ORCOUNTS rates are monitored (MAMA HV is off during this procedure).
- (2) Slow, intermediate voltage high-voltage ramp-up. The MCP HV is slow-ramped to a voltage 300V below nominal. A dark time-tag exposure is taken during this partial ramp. A second dark time-tag exposure is taken where the event counter is cycled through W, X, Y, Z, OR, EV and VE.
- (3) Ramp-up to full operating voltage. As before, a dark time-tag exposure is taken during this ramp-up. A second dark time-tag exposure is taken where the event counter is cycled through W, X, Y, Z, OR, EV and VE.
- (4) Fold analysis test (See COS TIR 2010-01).

In order for a recovery to be initiated the following conditions have to have been met:

- (1) MAMA HV shut down anomalously.
- (2) A minimum of 24 hours must have elapsed since the initial shutdown and the intermediate HV ramp-up (step two above).
- (3) The COS external shutter must be closed.

**ADDITIONAL COMMENTS**


This is not a requirement but it is desirable to have real-time engineering telemetry (MA return) during the execution of the first three visits.

Proposal 12724 - Visit 01 - COS NUV Detector Recovery After Anomalous Shutdown

Thu Jun 21 01:03:27 GMT 2012

**Visit**  
**Proposal 12724, Visit 01, completed**  
**Diagnostic Status: No Diagnostics**  
 Scientific Instruments: S/C  
 Special Requirements: GYRO MODE 3GOBAD; ON HOLD ; PARALLEL  
*Comments: NUV-MAMA recovery from anomalous shutdown signal processing electronics checkout procedure - Part 1. Must clear event flag 2 for the commanding to execute. Since no high voltage is involved, this visit may be scheduled within the 24 hour period following an anomalous HV shutdown. There are no exposures taken in this visit; only engineering telemetry is required. Refer to ISR STIS 98-03.*  
*On Hold Comments: To be used only after an anomalous shutdown of the NUV high voltage.*

#	Label	Target	Config,Mode,Aperture	Spectral Els.	Opt. Params.	Special Reqs.	Groups	Exp. Time/[Actual Dur.]	Orbit
1	LV and Signal Processing Check	DARK	S/C, DATA, NONE			SAA CONTOUR 32; SPEC COM INSTR ELHDTLVN_1; QASISTATES COS SI OPERATE OPERATE; QASISTATES COS NUV HOLD HOLD	Same Alignment in Visit 01	1005.0 Secs [==>]	[1]
<i>Comments: Special NUV LV turn on and check. Switch on LV power supply. Set nominal decode configuration. Set amplifier threshold to default (0.48V). Set software global monitor to nominal values. Collect a minimum of 30 telemetry points (OR counts). Set amplifier threshold to 0.28V. Collect a minimum of 30 telemetry points (OR Counts). Counts (W, X, Y, etc) are sampled by telemetry every 10 seconds for COS.</i>									
2	LV Off	DARK	S/C, DATA, NONE			SAA CONTOUR 32; SPEC COM INSTR RLLVTHDN	Same Alignment in Visit 01	30.0 Secs [==>]	[1]
<i>Comments: Turn NUV LV off. Use the nominal reconfiguration instruction.</i>									
3	Set Flag 2	DARK	S/C, DATA, NONE			SAA CONTOUR 32; SPEC COM INSTR ELFLAG2	Same Alignment in Visit 01	1.0 Secs [==>]	[1]
<i>Comments: Set COS event flag 2</i>									

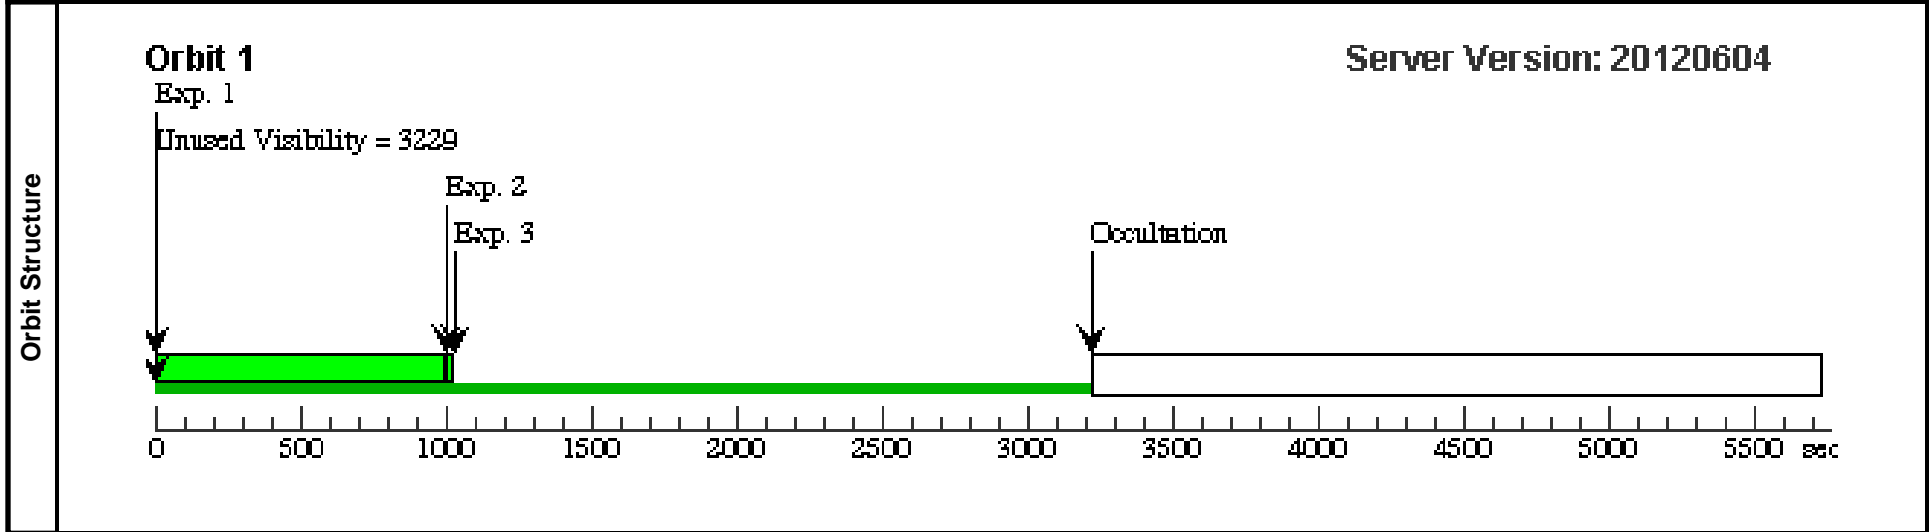

Proposal 12724 - Visit 02 - COS NUV Detector Recovery After Anomalous Shutdown


Visit	<p style="text-align: right;">Thu Jun 21 01:03:29 GMT 2012</p> <p><b>Proposal 12724, Visit 02, completed</b>  <b>Diagnostic Status: Warning</b>                  Scientific Instruments: COS/NUV, S/C                  Special Requirements: GYRO MODE 3GOBAD; AFTER 01 BY 12 H TO 36 H; ON HOLD ; PARALLEL  <i>Comments: NUV-MAMA recovery from anomalous shutdown intermediate voltage checkout procedure - Part 2.                  Must clear event flag 2 for the commanding to execute. Minimum wait of 24 hours following the anomalous shutdown. Goal: 1) Ramp NUV-MAMA to intermediate MCP voltage; 2) obtain dark count telemetry. Refer to ISR STIS 98-03.</i>  <i>On Hold Comments: To be used only after an anomalous shutdown of the NUV high voltage.</i></p>
Diagnostics	<p>(Visit 02) Warning (Orbit Planner): MAXIMUM DURATION EXCEEDED FOR INTERNAL OR EARTH CALIB SU</p>

# Proposal 12724 - Visit 02 - COS NUV Detector Recovery After Anomalous Shutdown

#	Label	Target	Config,Mode,Aperture	Spectral Els.	Opt. Params.	Special Reqs.	Groups	Exp. Time/[Actual Dur.]	Orbit
1	LV On	DARK	S/C, DATA, NONE			SAA CONTOUR 32; SPEC COM INSTR ELHDTLVN_2; QASISTATES COS SI OBSERVE OBSE RVE; QASISTATES COS NUV HOLD LVON	Sequence 1-6 Non-Int in Visit 02	60.0 Secs [==>]	[1]
<p><i>Comments: Special NUV LV turn on. Switch on LV power supply. Set nominal decode configuration. Set amplifier threshold to default (0.48V). Set software global monitor to nominal values.</i></p>									
2	Ramp HV to -1750/-50	DARK	COS/NUV, TIME-TAG, DEF	DEF	BUFFER-TIME=2000	SPEC COM INSTR ELLVTHVN_2; NEW ALIGNMENT ; QASISTATES COS SI OBSERVE OBSE RVE; QASISTATES COS NUV LVON HVON	Sequence 1-6 Non-Int in Visit 02	1800.0 Secs [==>]	[1]
<p><i>Comments: Special NUV HV turn on and slow partial HV ramp. The MCP and PC Voltage partial Ramp-ups will be performed in stages. The ramp-up within a stage is by increments of -50V. The final MCP voltage will be -1750V, 300V shy of the nominal value of -2050V. The final PC Voltage will be -50V, rather than the nominal -800V setting. Use the nominal yellow and red limits for ramping. At the end of each stage, reset the SGM to a Threshold = 100 and an Integration Period = 0.1 sec, and collect telemetry samples of OR Counts for 4 minutes. The COS rate is 1 TLM sample/10 secs; ~24 samples will be obtained. Stage 1 - MCP ramp-up (0 to -500V). Stage 2 - MCP ramp-up (-500V to -1000V). Stage 3 - MCP ramp-up (-1000V to -1500V). Stage 4 - MCP ramp-up (-1500V to -1750V). Stage 5 - PC Voltage ramp-up (+20 to -50V).</i></p>									
3	Cycle SGM	DARK	COS/NUV, TIME-TAG, DEF	DEF	BUFFER-TIME=720	SPEC COM INSTR ELHVDARK2; NEW ALIGNMENT	Sequence 1-6 Non-Int in Visit 02	570.0 Secs [==>]	[1]
<p><i>Comments: Special NUV DARK. Obtain an NUV DARK while at -1750V. During the exposure, set Software Global Monitor to an SGM Threshold = 200 and an Integration Period = 0.1 secs. Collect a minimum of 5 samples of W, X, Y, Z, OR, EV, and VE events. Because this is a COS exposure, the obset will end with a HOME Alignment. That HOME must have its COS NUV qasi_states reset via ISQL to have start_state = end_state = HOLD.</i></p>									
4	HV Off	DARK	S/C, DATA, NONE			SAA CONTOUR 32; SPEC COM INSTR ELHVTLVN_2; NEW ALIGNMENT ; QASISTATES COS SI OBSERVE OBSE RVE; QASISTATES COS NUV HVON LVON	Sequence 1-6 Non-Int in Visit 02	250.0 Secs [==>]	[1]
<p><i>Comments: Special NUV HV turn off. Ramp down PC &amp; MCP high voltage, and turn the HV off.</i></p>									

Proposal 12724 - Visit 02 - COS NUV Detector Recovery After Anomalous Shutdown

5	LV Off DARK S/C, DATA, NONE	SAA CONTOUR 32; Sequence 1-6 Non-In- t in Visit 02 SPEC COM INSTR RLLVTHDN; NEW ALIGNMENT ; QASISTATES COS SI OBSERVE OBSE RVE; QASISTATES COS NUV LVON HOLD	30.0 Secs [==>]	[1]
<p><i>Comments: Turn NUV LV off. Use the nominal reconfiguration instruction.</i></p>				
6	Set Flag 2 DARK S/C, DATA, NONE	SPEC COM INSTR Sequence 1-6 Non-In- t in Visit 02 ELFLAG2; NEW OBSET	1.0 Secs [==>]	[1]
<p><i>Comments: Set COS event flag 2. The NEW OBSET special requirement forces the HOME alignment to occur before this activity.</i></p>				

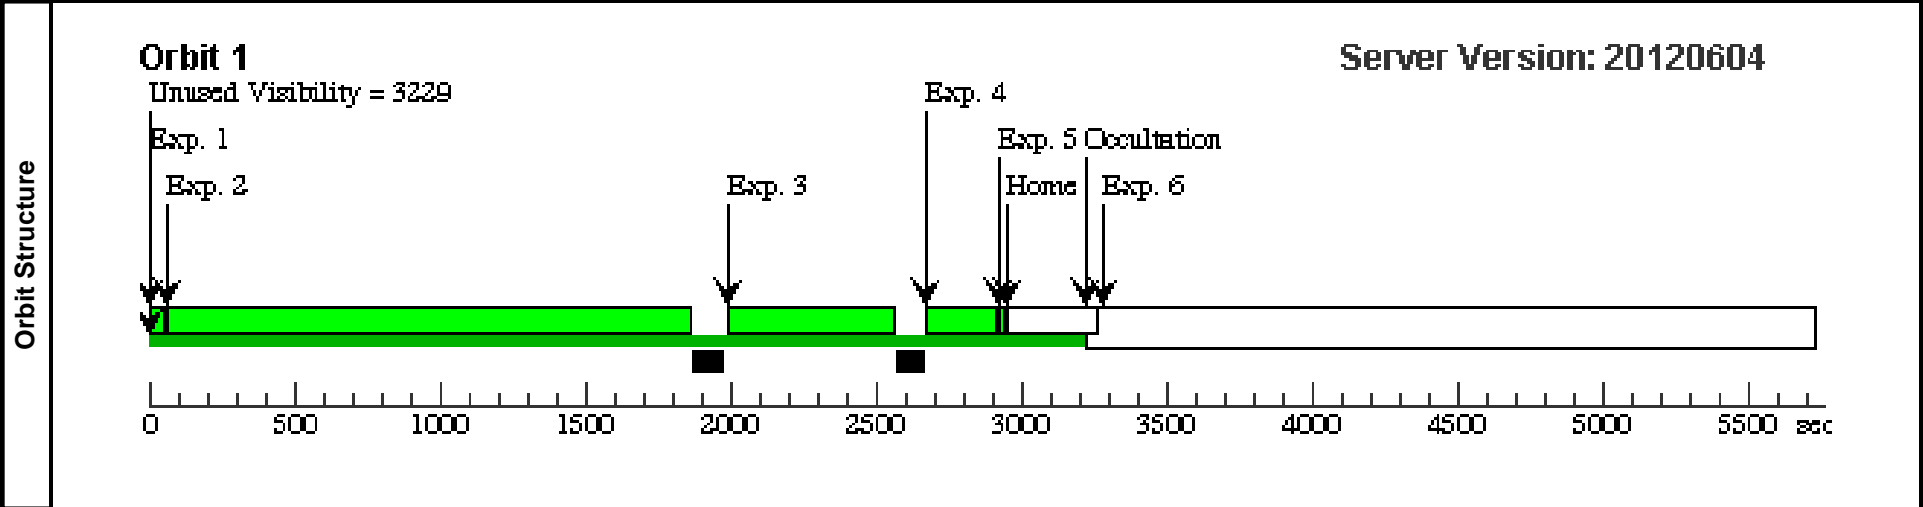

# Proposal 12724 - Visit 03 - COS NUV Detector Recovery After Anomalous Shutdown

<b>Visit</b>	<p><b>Proposal 12724, Visit 03, completed</b></p> <p><b>Diagnostic Status: Warning</b></p> <p>Scientific Instruments: COS/NUV, S/C</p> <p>Special Requirements: GYRO MODE 3GOBAD; AFTER 02 BY 24 H TO 48 H; ON HOLD ; PARALLEL</p> <p><i>Comments: NUV-MAMA recovery from anomalous shutdown nominal high voltage checkout procedure - Part 3.</i></p> <p><i>NSSC-1 COS event flag 2 must be clear for the commanding to execute.</i></p> <p><i>On Hold Comments: To be used only after an anomalous shutdown of the NUV high voltage.</i></p>	Thu Jun 21 01:03:30 GMT 2012
<b>Diagnostics</b>	(Visit 03) Warning (Orbit Planner): MAXIMUM DURATION EXCEEDED FOR INTERNAL OR EARTH CALIB SU	




# Proposal 12724 - Visit 03 - COS NUV Detector Recovery After Anomalous Shutdown

#	Label	Target	Config,Mode,Aperture	Spectral Els.	Opt. Params.	Special Reqs.	Groups	Exp. Time/[Actual Dur.]	Orbit
1	LV On	DARK	S/C, DATA, NONE			SAA CONTOUR 32; SPEC COM INSTR ELHDTLVN_3; QASISTATES COS SI OPERATE OBSE RVE; QASISTATES COS NUV HOLD LVON	Sequence 1-6 Non-Int in Visit 03	60.0 Secs [==>]	[1]
<p><i>Comments: Special NUV LV turn on. Switch on LV power supply. Set nominal decode configuration. Set amplifier threshold to default (0.48V). Set software global monitor to nominal values. Enable SDF.</i></p>									
2	Ramp HV to -2050/-800 (Nominal HV)	DARK	COS/NUV, TIME-TAG, DEF	DEF	BUFFER-TIME=33 00	SPEC COM INSTR ELLVTHVN_3; NEW ALIGNMENT ; QASISTATES COS SI OBSERVE OBSE RVE; QASISTATES COS NUV LVON HVON	Sequence 1-6 Non-Int in Visit 03	3090.0 Secs [==>]	[1]
<p><i>Comments: Special NUV HV turn on &amp; slow full ramp up. The MCP and Field Voltage Ramp-ups will be performed in stages. The ramp-up within a stage is by increments of 50V. Use the nominal yellow and red limits for ramping. At the end of each stage, reset the SGM to a Threshold = 100 and an Integration Period = 0.1 sec, and collect telemetry samples of Z Counts for 4 minutes. The COS rate is 1 TLM sample/10 secs; ~24 samples will be obtained. Stage 1 - MCP ramp-up (0 to -500V) Stage 2 - MCP ramp-up (-500V to -1000V) Stage 3 - MCP ramp-up (-1000V to -1500V) Stage 4 - MCP ramp-up (-1500V to -1750V) Stage 5 - PC Voltage ramp-up (+20 to -50V) Stage 6 - MCP ramp-up (-1750V to -1850V) Stage 7 - MCP ramp-up (-1850V to -1950V) Stage 8 - Final MCP ramp-up (-1950V to -2050V) Stage 9 - Final PC Voltage ramp-up (-50V to -800V)</i></p>									
3	Cycle SGM	DARK	COS/NUV, TIME-TAG, DEF	DEF	BUFFER-TIME=72 0	SPEC COM INSTR ELHVDARK3; NEW ALIGNMENT	Sequence 1-6 Non-Int in Visit 03	450.0 Secs [==>]	[1]
<p><i>Comments: Special NUV DARK. Obtain an NUV DARK while ramped up. During the exposure, set Software Global Monitor to an SGM Threshold = 200 and an Integration Period = 0.1 secs. Collect a minimum of 5 samples of W, X, Y, Z, OR, EV, and VE events. Because this is a COS exposure, the obset will end with a HOME Alignment. That HOME must have its COS NUV qasi_states reset via ISQL to have start_state = end_state = HOLD.</i></p>									
4	HV Off	DARK	S/C, DATA, NONE			SAA CONTOUR 32; SPEC COM INSTR ELHVTLVN_3; NEW ALIGNMENT ; QASISTATES COS SI OBSERVE OBSE RVE; QASISTATES COS NUV HVON LVON	Sequence 1-6 Non-Int in Visit 03	355.0 Secs [==>]	[1]
<p><i>Comments: Special NUV HV turn off. Ramp down PC &amp; MCP high voltage, and turn the HV off.</i></p>									

Proposal 12724 - Visit 03 - COS NUV Detector Recovery After Anomalous Shutdown


5	LV Off	DARK	S/C, DATA, NONE	SAA CONTOUR 32; Sequence 1-6 Non-In- SPEC COM INSTR t in Visit 03 RLLVTHDN; NEW ALIGNMENT ; QASISTATES COS SI OBSERVE OBSE RVE; QASISTATES COS NUV LVON HOLD	30.0 Secs [==>]	[1]
<p>Comments: Turn NUV LV off. Use the nominal reconfiguration instruction.</p>						
6	Set Flag 2	DARK	S/C, DATA, NONE	SPEC COM INSTR Sequence 1-6 Non-In- ELFLAG2; t in Visit 03 NEW OBSET	1.0 Secs [==>]	[1]
<p>Comments: Set COS event flag 2. The NEW OBSET special requirement forces the HOME alignment to occur before this activity.</p>						

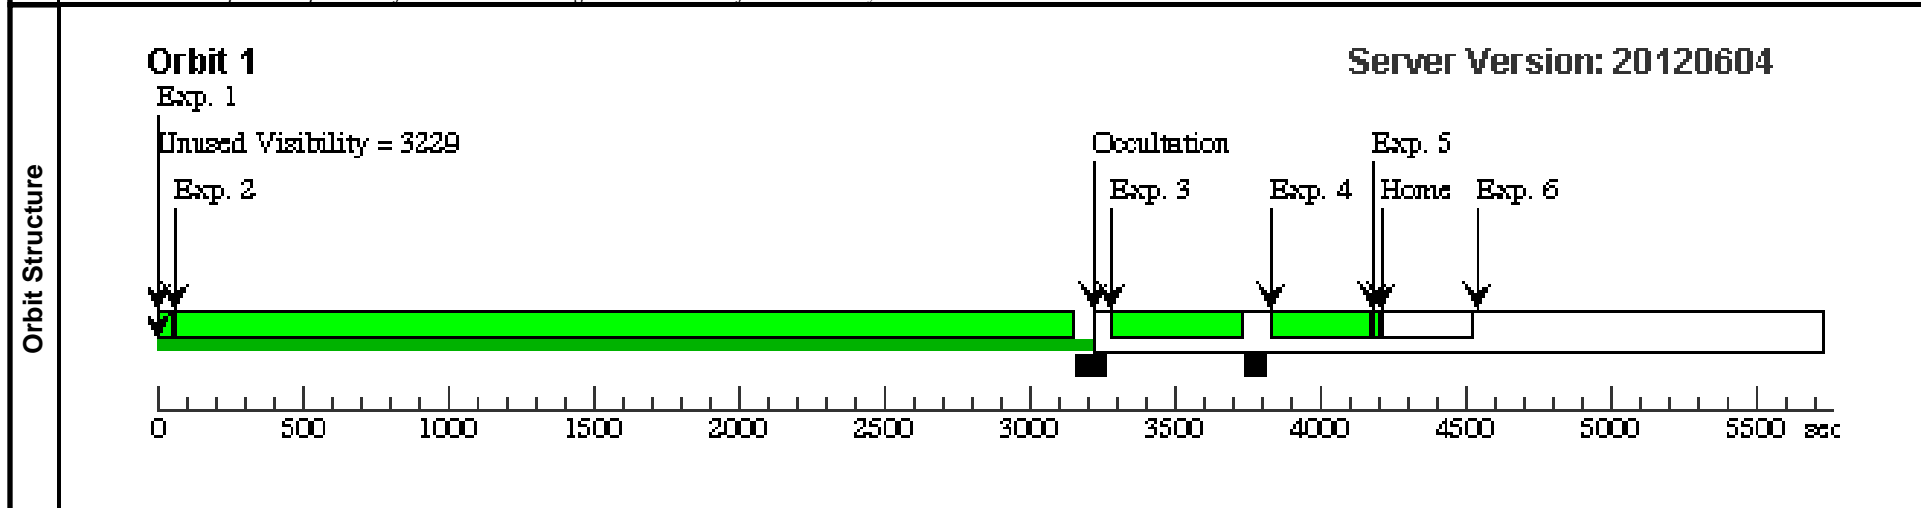

# Proposal 12724 - Visit 04 - COS NUV Detector Recovery After Anomalous Shutdown

Thu Jun 21 01:03:33 GMT 2012

Visit	<p><b>Proposal 12724, Visit 04, completed</b></p> <p><b>Diagnostic Status: Warning</b></p> <p>Scientific Instruments: COS/NUV, S/C</p> <p>Special Requirements: GYRO MODE 3GOBAD; AFTER 03 BY 24 H TO 48 H; ON HOLD ; PARALLEL</p> <p>Comments: NUV-MAMA recovery from anomalous shutdown Fold Distribution procedure - Part 4.</p> <p>On Hold Comments: To be used only after an anomalous shutdown of the NUV high voltage.</p>									
Diagnostics	<p>(Visit 04) Warning (Orbit Planner): MAXIMUM DURATION EXCEEDED FOR INTERNAL OR EARTH CALIB SU</p>									
Exposures	#	Label	Target	Config,Mode,Aperture	Spectral Els.	Opt. Params.	Special Reqs.	Groups	Exp. Time/[Actual Dur.]	Orbit
<p>1</p> <p>Fold Test Setup</p> <p>Comments: Special setup for NUV Fold Analysis Test. Set the Software Global Monitor to 150,000 ORCOUNTS per sec (sufficient to allow for spike at lamp turn-on).</p>	DARK	S/C, DATA, NONE			SAA CONTOUR 32; SPEC COM INSTR ELFOLDSET	Same Alignment in Visit 04	20.0 Secs [==>]	[1]		
	DEUTERIUM	COS/NUV, TIME-TAG, FCA	G185M 1850 A	CURRENT=MEDIU M; BUFFER-TIME=27 00	SPEC COM INSTR ELFOLDTST; QESIPARM TARG TYPE FOLD	Same Alignment in Visit 04	2300.0 Secs [==>]	[1]		
<p>Comments: Special NUV Fold Analysis Test. The FAT will be conducted during a deuterium lamp time-tag exposure. The exposure specification will ensure that the FCA aperture will be used, that the OSMs will be positioned at NCMIFLAT and G185M/1850, and that the lamp current is set to MEDIUM. Qesiparm TARGTYPE must be specified as FOLD so that the instructions will command the proper FAT lamp. Note that the FAT commanding will turn the lamp off during the exposure, and the exposure commanding will issue a redundant lamp off command after the exposure.</p> <p>Set Software Global monitor (SGM Threshold = 100000, SGM Integration period = 1 sec.)</p> <p>(a) Collect counter samples during flat field illumination. Collect 5 samples X events, Collect 5 samples Y events, Collect 5 samples Z events, Collect 5 samples W events, Collect 5 samples VE events, Collect 5 samples EV events, Collect 5 samples OR events. The TLM sample rate for COS is one sample / 10 seconds.</p> <p>(b) Disable MAMA Folds: C2, C3, C4, C5, C6, R2, R3, R4, R5, R6</p> <p>(c) Conduct fold analysis. Collect 5 samples VE for following 19 combinations of MAMA folds:</p> <p>(1) Enabled: C2, R2; Disabled: C3, C4, C5, C6, R3, R4, R5, R6</p> <p>(2) Enabled: C2, R3; Disabled: C3, C4, C5, C6, R2, R4, R5, R6</p> <p>(3) Enabled: C3, R2; Disabled: C2, C4, C5, C6, R3, R4, R5, R6</p> <p>(4) Enabled: C2, R4; Disabled: C3, C4, C5, C6, R2, R3, R5, R6</p> <p>(5) Enabled: C3, R3; Disabled: C2, C4, C5, C6, R2, R4, R5, R6</p> <p>(6) Enabled: C4, R2; Disabled: C2, C3, C5, C6, R3, R4, R5, R6</p> <p>(7) Enabled: C3, R4; Disabled: C2, C4, C5, C6, R2, R3, R5, R6</p> <p>(8) Enabled: C4, R3; Disabled: C2, C3, C5, C6, R2, R4, R5, R6</p> <p>(9) Enabled: C3, R5; Disabled: C2, C4, C5, C6, R2, R3, R4, R6</p> <p>(10) Enabled: C4, R4; Disabled: C2, C3, C5, C6, R2, R3, R5, R6</p> <p>(11) Enabled: C5, R3; Disabled: C2, C3, C4, C6, R2, R4, R5, R6</p> <p>(12) Enabled: C4, R5; Disabled: C2, C3, C5, C6, R2, R3, R4, R6</p> <p>(13) Enabled: C5, R4; Disabled: C2, C3, C4, C6, R2, R3, R5, R6</p> <p>(14) Enabled: C4, R6; Disabled: C2, C3, C5, C6, R2, R3, R4, R5</p> <p>(15) Enabled: C5, R5; Disabled: C2, C3, C4, C6, R2, R3, R4, R6</p> <p>(16) Enabled: C6, R4; Disabled: C2, C3, C4, C5, R2, R3, R5, R6</p> <p>(17) Enabled: C5, R6; Disabled: C2, C3, C4, C6, R2, R3, R4, R5</p> <p>(18) Enabled: C6, R5; Disabled: C2, C3, C4, C5, R2, R3, R4, R6</p> <p>(19) Enabled: C6, R6; Disabled: C2, C3, C4, C5, R2, R3, R4, R5</p> <p>(d) Enable MAMA folds C2, C3, C4, C5, C6, R2, R3, R4, R5, R6</p> <p>(e) Check lamp stability by checking EV and VE: Collect 5 samples events (EV). Collect 5 samples Valid Events (VE)</p> <p>(f) Turn off the FAT lamp</p> <p>(g) Collect event counter data for detector dark count rate. Collect 5 samples X dark events. Collect 5 samples Y dark events. Collect 5 samples Z dark events. Collect 5 samples W dark events. Collect 5 samples VE dark events. Collect 5 samples EV dark events. Collect 5 samples OR dark events</p> <p>(h) At completion of procedure reset SGM to nominal operating level</p>										

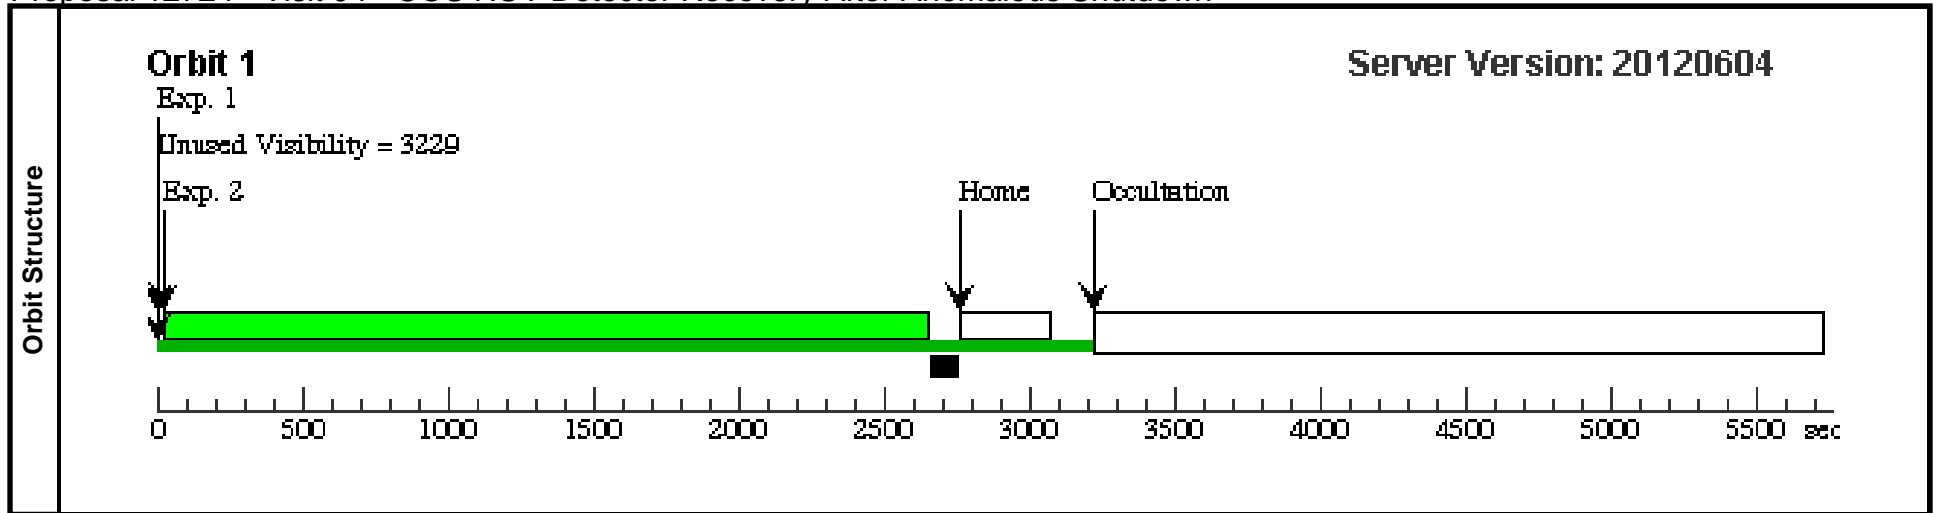


Proposal 12724 - Signal Processing Electronics Checkout (11) - COS NUV Detector Recovery After Anomalous Shutdown

Thu Jun 21 01:03:34 GMT 2012

**Visit**  
**Proposal 12724, Signal Processing Electronics Checkout (11)**  
**Diagnostic Status: No Diagnostics**  
 Scientific Instruments: S/C  
 Special Requirements: GYRO MODE 3GOBAD; ON HOLD ; PARALLEL  
*Comments: NUV-MAMA recovery from anomalous shutdown signal processing electronics checkout procedure - Part 1. Must clear event flag 2 for the commanding to execute. Since no high voltage is involved, this visit may be scheduled within the 24 hour period following an anomalous HV shutdown. There are no exposures taken in this visit; only engineering telemetry is required. Refer to ISR STIS 98-03.*  
*On Hold Comments: To be used only after an anomalous shutdown of the NUV high voltage.*

#	Label	Target	Config,Mode,Aperture	Spectral Els.	Opt. Params.	Special Reqs.	Groups	Exp. Time/[Actual Dur.]	Orbit
1	LV and Signal Processing Check	DARK	S/C, DATA, NONE			SAA CONTOUR 32; SPEC COM INSTR ELHDTLVN_1; QASISTATES COS SI OPERATE OPERATE; QASISTATES COS NUV HOLD HOLD	Same Alignment in Signal Processing Electronics Checkout (11)	1005.0 Secs [==>]	[1]
<i>Comments: Special NUV LV turn on and check. Switch on LV power supply. Set nominal decode configuration. Set amplifier threshold to default (0.48V). Set software global monitor to nominal values. Collect a minimum of 30 telemetry points (OR counts). Set amplifier threshold to 0.28V. Collect a minimum of 30 telemetry points (OR Counts). Counts (W, X, Y, etc) are sampled by telemetry every 10 seconds for COS.</i>									
2	LV Off	DARK	S/C, DATA, NONE			SAA CONTOUR 32; SPEC COM INSTR RLLVTHDN	Same Alignment in Signal Processing Electronics Checkout (11)	30.0 Secs [==>]	[1]
<i>Comments: Turn NUV LV off. Use the nominal reconfiguration instruction.</i>									
3	Set Flag 2	DARK	S/C, DATA, NONE			SAA CONTOUR 32; SPEC COM INSTR ELFLAG2	Same Alignment in Signal Processing Electronics Checkout (11)	1.0 Secs [==>]	[1]
<i>Comments: Set COS event flag 2</i>									

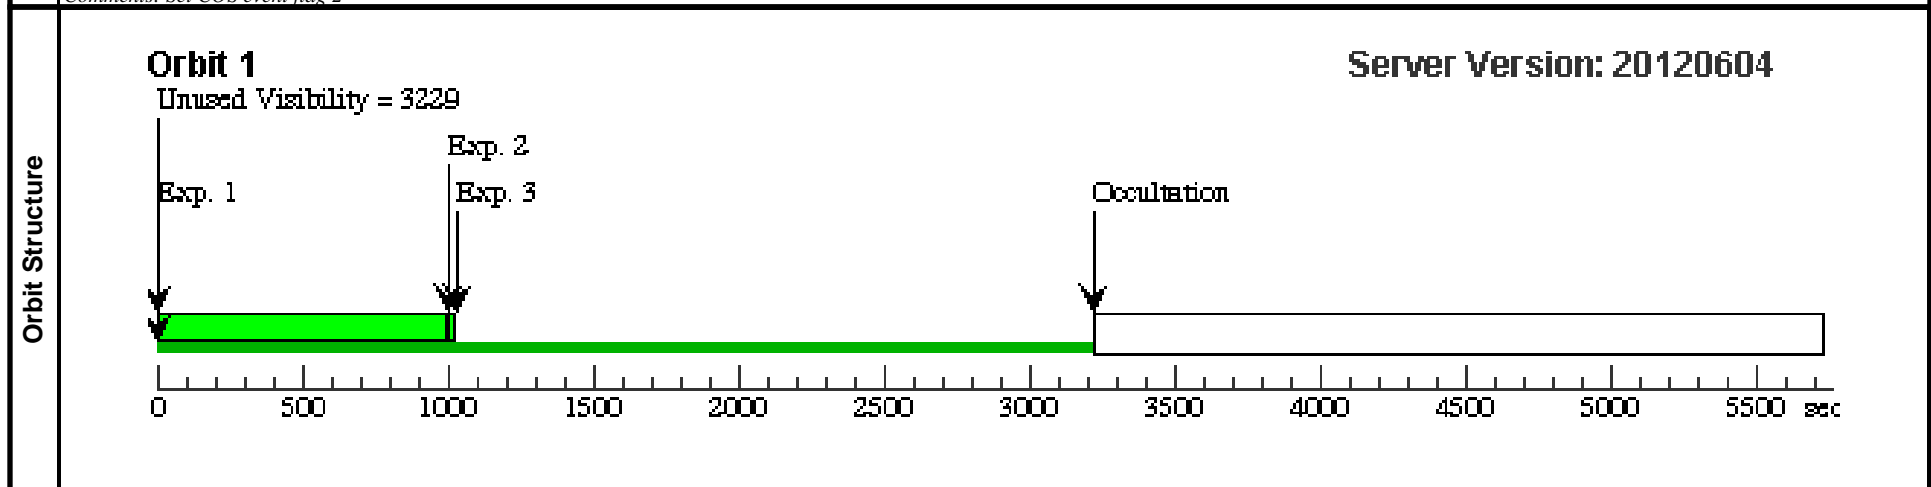

Proposal 12724 - Ramp HV to Intermediate HV (-1750/-50) (12) - COS NUV Detector Recovery After Anomalous Shutdown


<b>Visit</b>	<p style="text-align: right;">Thu Jun 21 01:03:34 GMT 2012</p> <p><b>Proposal 12724, Ramp HV to Intermediate HV (-1750/-50) (12)</b>  <b>Diagnostic Status: Warning</b>                  Scientific Instruments: COS/NUV, S/C                  Special Requirements: GYRO MODE 3GOBAD; AFTER 11 BY 12 H TO 36 H; ON HOLD ; PARALLEL  <i>Comments: NUV-MAMA recovery from anomalous shutdown intermediate voltage checkout procedure - Part 2.                  Must clear event flag 2 for the commanding to execute. Minimum wait of 24 hours following the anomalous shutdown. Goal: 1) Ramp NUV-MAMA to intermediate MCP voltage; 2) obtain dark count telemetry. Refer to ISR STIS 98-03.</i>  <i>On Hold Comments: To be used only after an anomalous shutdown of the NUV high voltage.</i></p>
<b>Diagnostics</b>	<p>(Ramp HV to Intermediate HV (-1750/-50) (12)) Warning (Orbit Planner): MAXIMUM DURATION EXCEEDED FOR INTERNAL OR EARTH CALIB SU</p>

Proposal 12724 - Ramp HV to Intermediate HV (-1750/-50) (12) - COS NUV Detector Recovery After Anomalous Shutdown

#	Label	Target	Config,Mode,Aperture	Spectral Els.	Opt. Params.	Special Reqs.	Groups	Exp. Time/[Actual Dur.]	Orbit
1	LV On	DARK	S/C, DATA, NONE			SAA CONTOUR 32; SPEC COM INSTR ELHDTLVN_2; QASISTATES COS SI OBSERVE OBSE RVE; QASISTATES COS NUV HOLD LVON	Sequence 1-6 Non-Int in Ramp HV to Intermediate HV (-1750/-50) (12)	60.0 Secs [==>]	[1]
<p>Comments: Special NUV LV turn on. Switch on LV power supply. Set nominal decode configuration. Set amplifier threshold to default (0.48V). Set software global monitor to nominal values.</p>									
2	Ramp HV to -1750/-50	DARK	COS/NUV, TIME-TAG, DEF	DEF	BUFFER-TIME=2000	SPEC COM INSTR ELLVTHVN_2; NEW ALIGNMENT ; QASISTATES COS SI OBSERVE OBSE RVE; QASISTATES COS NUV LVON HVON	Sequence 1-6 Non-Int in Ramp HV to Intermediate HV (-1750/-50) (12)	1800.0 Secs [==>]	[1]
<p>Comments: Special NUV HV turn on and slow partial HV ramp. The MCP and PC Voltage partial Ramp-ups will be performed in stages. The ramp-up within a stage is by increments of -50V. The final MCP voltage will be -1750V, 300V shy of the nominal value of -2050V. The final PC Voltage will be -50V, rather than the nominal -800V setting. Use the nominal yellow and red limits for ramping. At the end of each stage, reset the SGM to a Threshold = 100 and an Integration Period = 0.1 sec, and collect telemetry samples of OR Counts for 4 minutes. The COS rate is 1 TLM sample/10 secs; ~24 samples will be obtained. Stage 1 - MCP ramp-up (0 to -500V). Stage 2 - MCP ramp-up (-500V to -1000V). Stage 3 - MCP ramp-up (-1000V to -1500V). Stage 4 - MCP ramp-up (-1500V to -1750V). Stage 5 - PC Voltage ramp-up (+20 to -50V).</p>									
3	Cycle SGM	DARK	COS/NUV, TIME-TAG, DEF	DEF	BUFFER-TIME=720	SPEC COM INSTR ELHVDARK2; NEW ALIGNMENT	Sequence 1-6 Non-Int in Ramp HV to Intermediate HV (-1750/-50) (12)	570.0 Secs [==>]	[1]
<p>Comments: Special NUV DARK. Obtain an NUV DARK while at -1750V. During the exposure, set Software Global Monitor to an SGM Threshold = 200 and an Integration Period = 0.1 secs. Collect a minimum of 5 samples of W, X, Y, Z, OR, EV, and VE events. Because this is a COS exposure, the obset will end with a HOME Alignment. That HOME must have its COS NUV qasi_states reset via ISQL to have start_state = end_state = HOLD.</p>									
4	HV Off	DARK	S/C, DATA, NONE			SAA CONTOUR 32; SPEC COM INSTR ELHVTLVN_2; NEW ALIGNMENT ; QASISTATES COS SI OBSERVE OBSE RVE; QASISTATES COS NUV HVON LVON	Sequence 1-6 Non-Int in Ramp HV to Intermediate HV (-1750/-50) (12)	250.0 Secs [==>]	[1]
<p>Comments: Special NUV HV turn off. Ramp down PC &amp; MCP high voltage, and turn the HV off.</p>									

Proposal 12724 - Ramp HV to Intermediate HV (-1750/-50) (12) - COS NUV Detector Recovery After Anomalous Shutdown

5	LV Off	DARK	S/C, DATA, NONE	SAA CONTOUR 32; Sequence 1-6 Non-Int in Ramp HV to Inter- mediate HV (-1750/ -50) (12)  SPEC COM INSTR RLLVTHDN;  NEW ALIGNMENT ;  QASISTATES COS SI OBSERVE OBSE RVE;  QASISTATES COS NUV LVON HOLD	30.0 Secs [==>]	[!]	
<i>Comments: Turn NUV LV off. Use the nominal reconfiguration instruction.</i>							
6	Set Flag 2	DARK	S/C, DATA, NONE	SPEC COM INSTR ELFLAG2; NEW OBSET	Sequence 1-6 Non-Int in Ramp HV to Inter- mediate HV (-1750/ -50) (12) 1.0 Secs [==>]	[!]	
<i>Comments: Set COS event flag 2. The NEW OBSET special requirement forces the HOME alignment to occur before this activity.</i>							

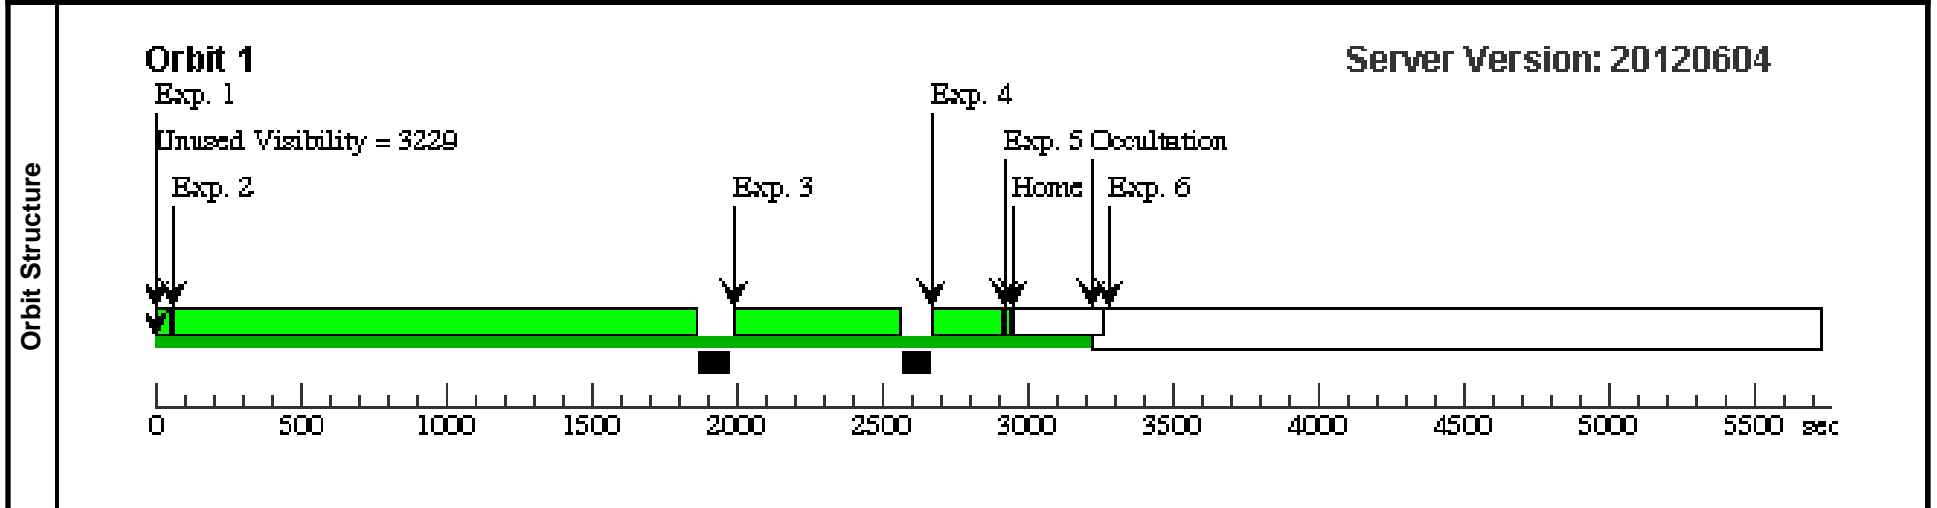



Proposal 12724 - Ramp HV to Nominal HV (-2050/-800) (13) - COS NUV Detector Recovery After Anomalous Shutdown


<b>Visit</b>	<p style="text-align: right;">Thu Jun 21 01:03:35 GMT 2012</p> <p><b>Proposal 12724, Ramp HV to Nominal HV (-2050/-800) (13)</b>  <b>Diagnostic Status: Warning</b>                  Scientific Instruments: COS/NUV, S/C                  Special Requirements: GYRO MODE 3GOBAD; AFTER 12 BY 24 H TO 48 H; ON HOLD ; PARALLEL  <i>Comments: NUV-MAMA recovery from anomalous shutdown nominal high voltage checkout procedure - Part 3.</i>  <i>NSSC-1 COS event flag 2 must be clear for the commanding to execute.</i>  <i>On Hold Comments: To be used only after an anomalous shutdown of the NUV high voltage.</i></p>
<b>Diagnostics</b>	<p>(Ramp HV to Nominal HV (-2050/-800) (13)) Warning (Orbit Planner): MAXIMUM DURATION EXCEEDED FOR INTERNAL OR EARTH CALIB SU</p>

Proposal 12724 - Ramp HV to Nominal HV (-2050/-800) (13) - COS NUV Detector Recovery After Anomalous Shutdown

#	Label	Target	Config,Mode,Aperture	Spectral Els.	Opt. Params.	Special Reqs.	Groups	Exp. Time/[Actual Dur.]	Orbit
1	LV On	DARK	S/C, DATA, NONE			SAA CONTOUR 32; SPEC COM INSTR ELHDTLVN_3; QASISTATES COS SI OPERATE OBSE RVE; QASISTATES COS NUV HOLD LVON	Sequence 1-6 Non-Int in Ramp HV to Nominal HV (-2050/-800) (13)	60.0 Secs [==>]	[1]
<p>Comments: Special NUV LV turn on. Switch on LV power supply. Set nominal decode configuration. Set amplifier threshold to default (0.48V). Set software global monitor to nominal values. Enable SDF.</p>									
2	Ramp HV to -2050/-800 (Nominal HV)	DARK	COS/NUV, TIME-TAG, DEF	DEF	BUFFER-TIME=3300	SPEC COM INSTR ELLVTHVN_3; NEW ALIGNMENT ; QASISTATES COS SI OBSERVE OBSE RVE; QASISTATES COS NUV LVON HVON	Sequence 1-6 Non-Int in Ramp HV to Nominal HV (-2050/-800) (13)	3090.0 Secs [==>]	[1]
<p>Comments: Special NUV HV turn on &amp; slow full ramp up. The MCP and Field Voltage Ramp-ups will be performed in stages. The ramp-up within a stage is by increments of 50V. Use the nominal yellow and red limits for ramping. At the end of each stage, reset the SGM to a Threshold = 1000 and an Integration Period = 0.1 sec, and collect telemetry samples of Z Counts for 4 minutes. The COS rate is 1 TLM sample/10 secs; ~24 samples will be obtained. Stage 1 - MCP ramp-up (0 to -500V) Stage 2 - MCP ramp-up (-500V to -1000V) Stage 3 - MCP ramp-up (-1000V to -1500V) Stage 4 - MCP ramp-up (-1500V to -1750V) Stage 5 - PC Voltage ramp-up (+20 to -50V) Stage 6 - MCP ramp-up (-1750V to -1850V) Stage 7 - MCP ramp-up (-1850V to -1950V) Stage 8 - Final MCP ramp-up (-1950V to -2050V) Stage 9 - Final PC Voltage ramp-up (-50V to -800V)</p>									
3	Cycle SGM	DARK	COS/NUV, TIME-TAG, DEF	DEF	BUFFER-TIME=720	SPEC COM INSTR ELHVDARK3; NEW ALIGNMENT	Sequence 1-6 Non-Int in Ramp HV to Nominal HV (-2050/-800) (13)	450.0 Secs [==>]	[1]
<p>Comments: Special NUV DARK. Obtain an NUV DARK while ramped up. During the exposure, set Software Global Monitor to an SGM Threshold = 200 and an Integration Period = 0.1 secs. Collect a minimum of 5 samples of W, X, Y, Z, OR, EV, and VE events. Because this is a COS exposure, the obset will end with a HOME Alignment. That HOME must have its COS NUV qasi_states reset via ISQL to have start_state = end_state = HOLD.</p>									
4	HV Off	DARK	S/C, DATA, NONE			SAA CONTOUR 32; SPEC COM INSTR ELHVTLVN_3; NEW ALIGNMENT ; QASISTATES COS SI OBSERVE OBSE RVE; QASISTATES COS NUV HVON LVON	Sequence 1-6 Non-Int in Ramp HV to Nominal HV (-2050/-800) (13)	355.0 Secs [==>]	[1]
<p>Comments: Special NUV HV turn off. Ramp down PC &amp; MCP high voltage, and turn the HV off.</p>									

Proposal 12724 - Ramp HV to Nominal HV (-2050/-800) (13) - COS NUV Detector Recovery After Anomalous Shutdown

5	LV Off	DARK	S/C, DATA, NONE	SAA CONTOUR 32; Sequence 1-6 Non-Int in Ramp HV to Nominal HV (-2050/-800) (13) SPEC COM INSTR RLLVTHDN; NEW ALIGNMENT ; QASISTATES COS SI OBSERVE OBSE RVE; QASISTATES COS NUV LVON HOLD	30.0 Secs [==>]	[1]
Comments: Turn NUV LV off. Use the nominal reconfiguration instruction.						
6	Set Flag 2	DARK	S/C, DATA, NONE	SPEC COM INSTR ELFLAG2; NEW OBSET	1.0 Secs [==>]	[1]
Comments: Set COS event flag 2. The NEW OBSET special requirement forces the HOME alignment to occur before this activity.						

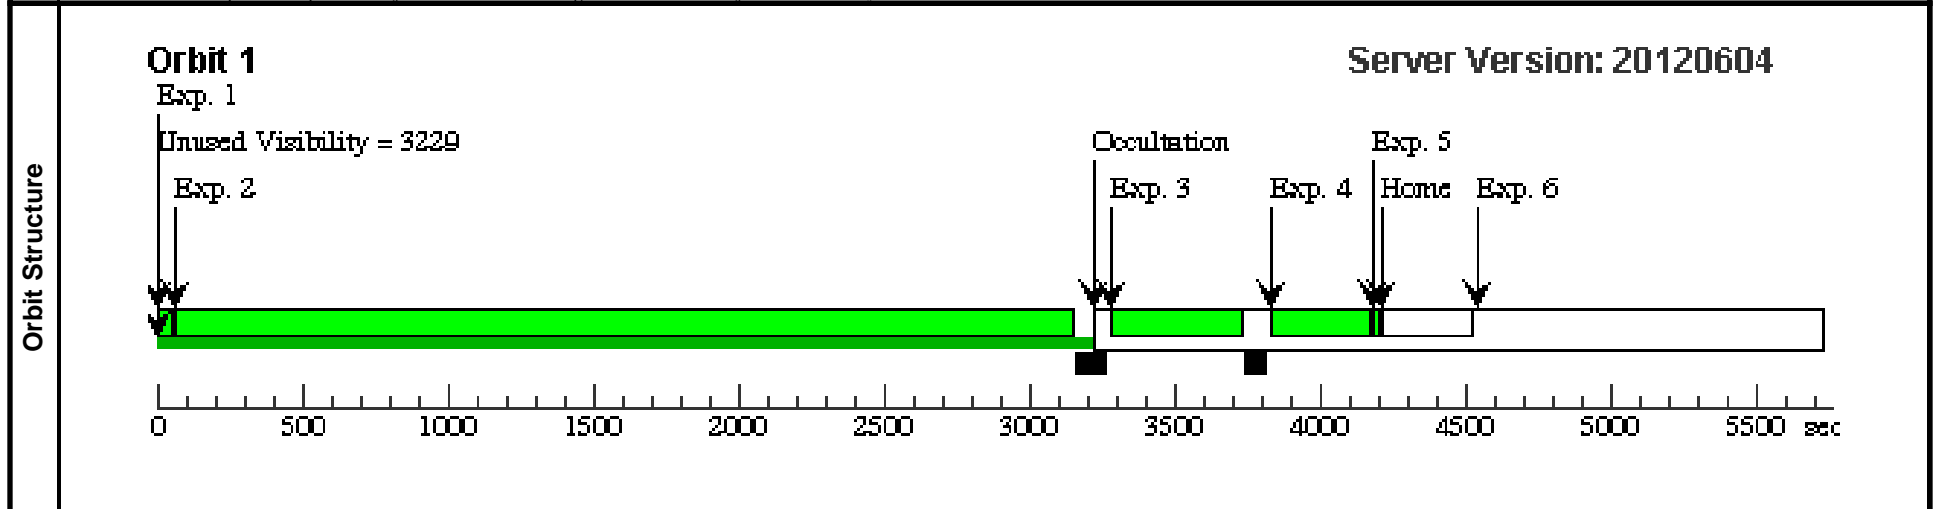

Proposal 12724 - Fold Distribution Test (14) - COS NUV Detector Recovery After Anomalous Shutdown

Thu Jun 21 01:03:36 GMT 2012

<b>Visit</b>	<p><b>Proposal 12724, Fold Distribution Test (14)</b></p> <p><b>Diagnostic Status: Warning</b></p> <p>Scientific Instruments: COS/NUV, S/C</p> <p>Special Requirements: GYRO MODE 3GOBAD; AFTER 13 BY 24 H TO 48 H; ON HOLD ; PARALLEL</p> <p>Comments: NUV-MAMA recovery from anomalous shutdown Fold Distribution procedure - Part 4.</p> <p>On Hold Comments: To be used only after an anomalous shutdown of the NUV high voltage.</p>									
	<p>(Fold Distribution Test (14)) Warning (Orbit Planner): MAXIMUM DURATION EXCEEDED FOR INTERNAL OR EARTH CALIB SU</p>									
<b>Diagnostics</b>										
<b>Exposures</b>	<b>#</b>	<b>Label</b>	<b>Target</b>	<b>Config,Mode,Aperture</b>	<b>Spectral Els.</b>	<b>Opt. Params.</b>	<b>Special Reqs.</b>	<b>Groups</b>	<b>Exp. Time/[Actual Dur.]</b>	<b>Orbit</b>
	1	Fold Test Setup	DARK	S/C, DATA, NONE			SAA CONTOUR 32; SPEC COM INSTR ELFOLDSET	Same Alignment in Fold Distribution Test (14)	20.0 Secs [==>]	[1]
<p>Comments: Special setup for NUV Fold Analysis Test. Set the Software Global Monitor to 150,000 ORCOUNTS per sec (sufficient to allow for spike at lamp turn-on).</p>										
2	Fold Test	DEUTERIUM	COS/NUV, TIME-TAG, FCA	G185M 1850 A	CURRENT=MEDIUM; BUFFER-TIME=2700	SPEC COM INSTR ELFOLDTST; QESIPARM TARG TYPE FOLD	Same Alignment in Fold Distribution Test (14)	2300.0 Secs [==>]	[1]	
<p>Comments: Special NUV Fold Analysis Test. The FAT will be conducted during a deuterium lamp time-tag exposure. The exposure specification will ensure that the FCA aperture will be used, that the OSMs will be positioned at NCMIFLAT and G185M/1850, and that the lamp current is set to MEDIUM. Qesiparm TARGTYPE must be specified as FOLD so that the instructions will command the proper FAT lamp. Note that the FAT commanding will turn the lamp off during the exposure, and the exposure commanding will issue a redundant lamp off command after the exposure.</p> <p>Set Software Global monitor (SGM Threshold = 100000, SGM Integration period = 1 sec.)</p> <p>(a) Collect counter samples during flat field illumination. Collect 5 samples X events, Collect 5 samples Y events, Collect 5 samples Z events, Collect 5 samples W events, Collect 5 samples VE events, Collect 5 samples EV events, Collect 5 samples OR events. The TLM sample rate for COS is one sample / 10 seconds.</p> <p>(b) Disable MAMA Folds: C2, C3, C4, C5, C6, R2, R3, R4, R5, R6</p> <p>(c) Conduct fold analysis. Collect 5 samples VE for following 19 combinations of MAMA folds:</p> <p>(1) Enabled: C2, R2; Disabled: C3, C4, C5, C6, R3, R4, R5, R6</p> <p>(2) Enabled: C2, R3; Disabled: C3, C4, C5, C6, R2, R4, R5, R6</p> <p>(3) Enabled: C3, R2; Disabled: C2, C4, C5, C6, R3, R4, R5, R6</p> <p>(4) Enabled: C2, R4; Disabled: C3, C4, C5, C6, R2, R3, R5, R6</p> <p>(5) Enabled: C3, R3; Disabled: C2, C4, C5, C6, R2, R4, R5, R6</p> <p>(6) Enabled: C4, R2; Disabled: C2, C3, C5, C6, R3, R4, R5, R6</p> <p>(7) Enabled: C3, R4; Disabled: C2, C4, C5, C6, R2, R3, R5, R6</p> <p>(8) Enabled: C4, R3; Disabled: C2, C3, C5, C6, R2, R4, R5, R6</p> <p>(9) Enabled: C3, R5; Disabled: C2, C4, C5, C6, R2, R3, R4, R6</p> <p>(10) Enabled: C4, R4; Disabled: C2, C3, C5, C6, R2, R3, R5, R6</p> <p>(11) Enabled: C5, R3; Disabled: C2, C3, C4, C6, R2, R4, R5, R6</p> <p>(12) Enabled: C4, R5; Disabled: C2, C3, C5, C6, R2, R3, R4, R6</p> <p>(13) Enabled: C5, R4; Disabled: C2, C3, C4, C6, R2, R3, R5, R6</p> <p>(14) Enabled: C4, R6; Disabled: C2, C3, C5, C6, R2, R3, R4, R5</p> <p>(15) Enabled: C5, R5; Disabled: C2, C3, C4, C6, R2, R3, R4, R6</p> <p>(16) Enabled: C6, R4; Disabled: C2, C3, C4, C5, R2, R3, R5, R6</p> <p>(17) Enabled: C5, R6; Disabled: C2, C3, C4, C6, R2, R3, R4, R5</p> <p>(18) Enabled: C6, R5; Disabled: C2, C3, C4, C5, R2, R3, R4, R6</p> <p>(19) Enabled: C6, R6; Disabled: C2, C3, C4, C5, R2, R3, R4, R5</p> <p>(d) Enable MAMA folds C2, C3, C4, C5, C6, R2, R3, R4, R5, R6</p> <p>(e) Check lamp stability by checking EV and VE: Collect 5 samples events (EV). Collect 5 samples Valid Events (VE)</p> <p>(f) Turn off the FAT lamp</p> <p>(g) Collect event counter data for detector dark count rate. Collect 5 samples X dark events. Collect 5 samples Y dark events. Collect 5 samples Z dark events. Collect 5 samples W dark events. Collect 5 samples VE dark events. Collect 5 samples EV dark events. Collect 5 samples OR dark events</p> <p>(h) At completion of procedure reset SGM to nominal operating level</p>										

