

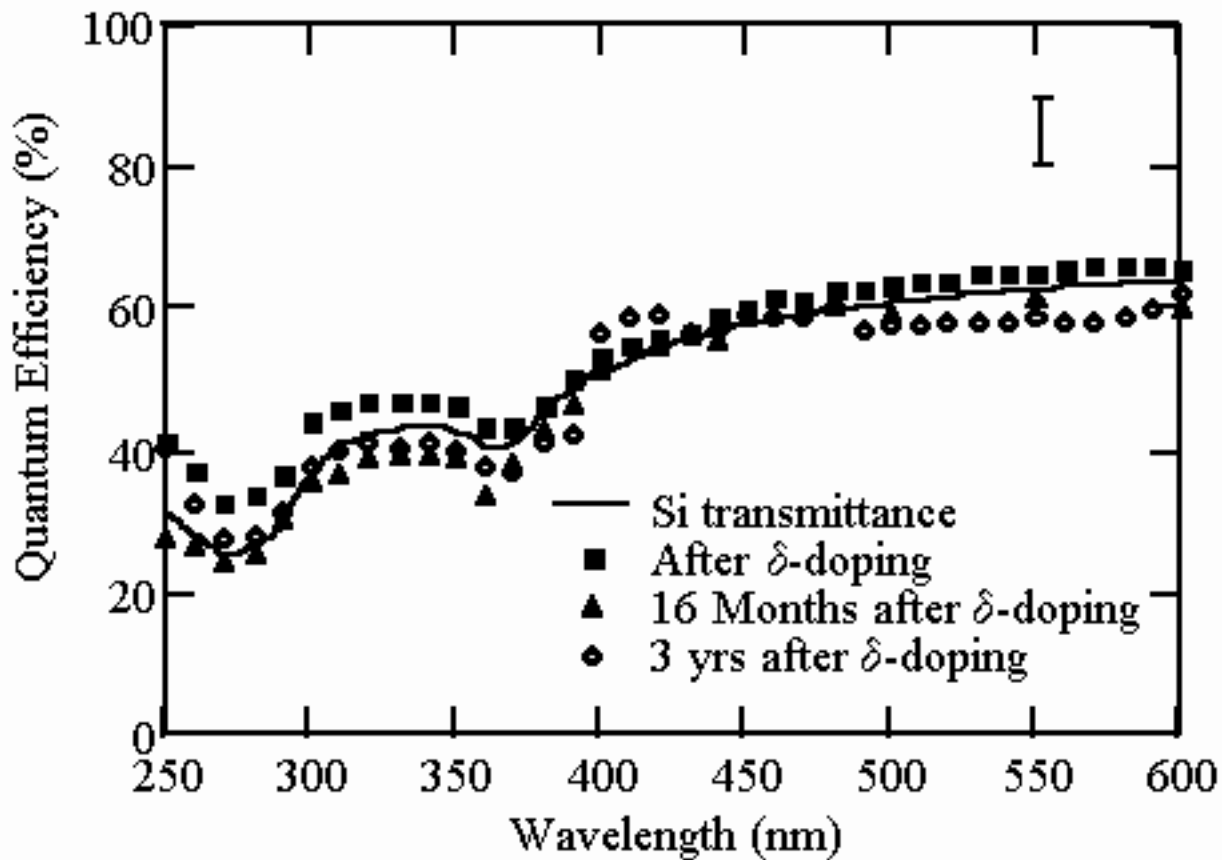
Figure 3

Figure 3. QE measured over a three-year period on the same delta-doped CCD. The CCD was stored unprotected in a laboratory environment. The error bars represent the accuracy ($\pm 5\%$) of the measurement systems used.